


Shodex™

Capture the Essence



2018-2019

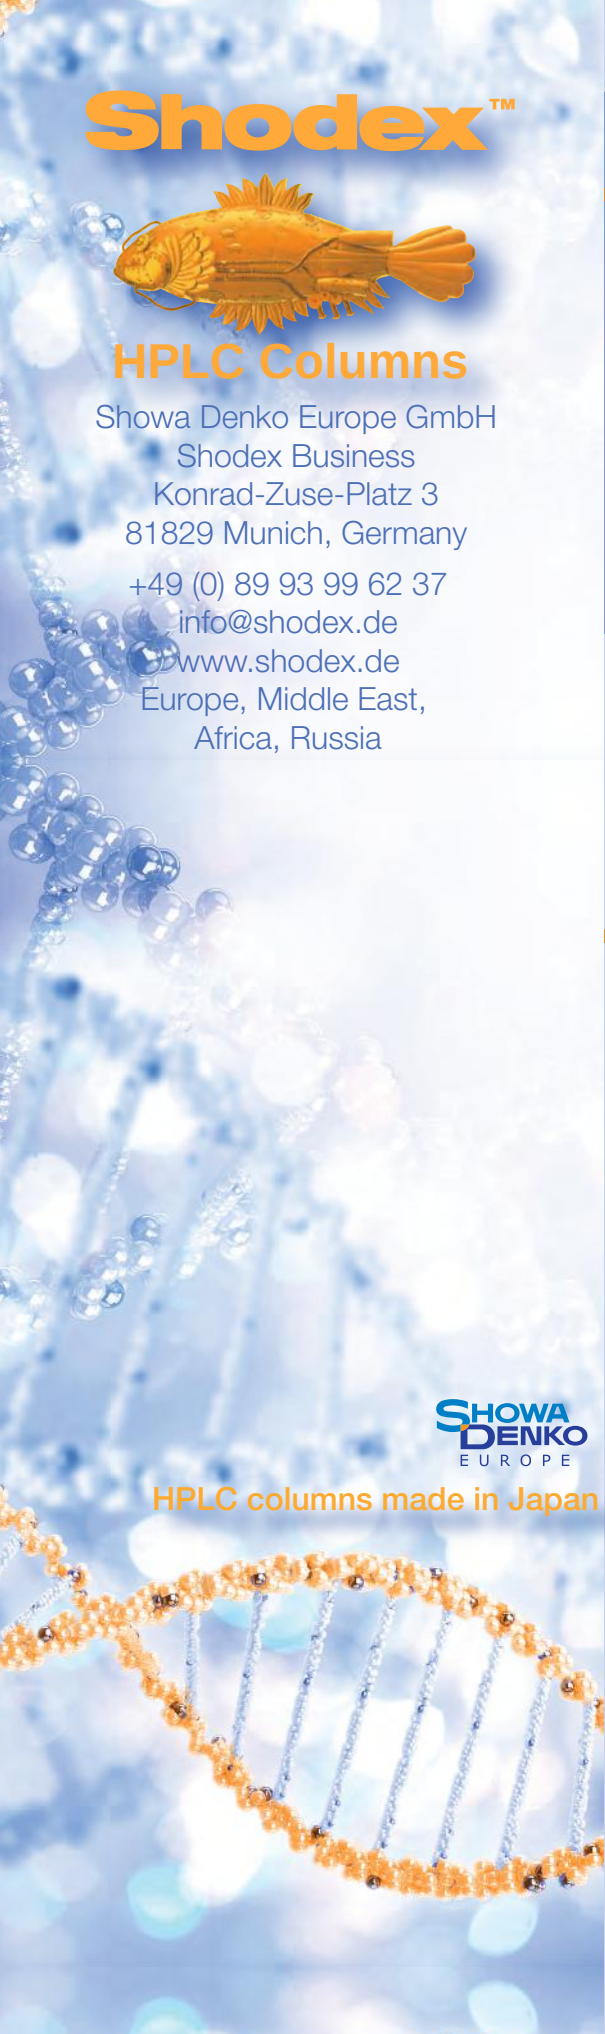

Shodex™

HPLC Columns

Showa Denko Europe GmbH

Shodex Business

Konrad-Zuse-Platz 3

81829 Munich, Germany

+49 (0) 89 93 99 62 37

info@shodex.de

www.shodex.de

Europe, Middle East,

Africa, Russia

**SHOWA
DENKO**
EUROPE

HPLC columns made in Japan

Why to buy polymer-based columns?


- ✱ The great chemical stability leads to an extended pH range (2 to 13).
- ✱ The low bleeding allows the use of sensitive detection.
- ✱ The large variety of material properties creates a higher resolution.
- ✱ They are available for almost all separation techniques.
- ✱ The price per injection is cheaper than in silica-based columns due to their extended lifetime (2 to 3 times longer than silica-based).

Why to choose Shodex as supplier?

- ✱ We offer a comprehensive and high standard technical support (pre- and after-sales).
- ✱ We provide 50 years of experience.
- ✱ Our experience leads to a great knowledge and a huge application database.
- ✱ Full production control: own production of polymer gels & own column packing.
- ✱ Strong partnership with customers and distributors.
- ✱ We offer you demo columns for free during 30 days.

Register on our new website and get
lots more of information:

www.shodex.de

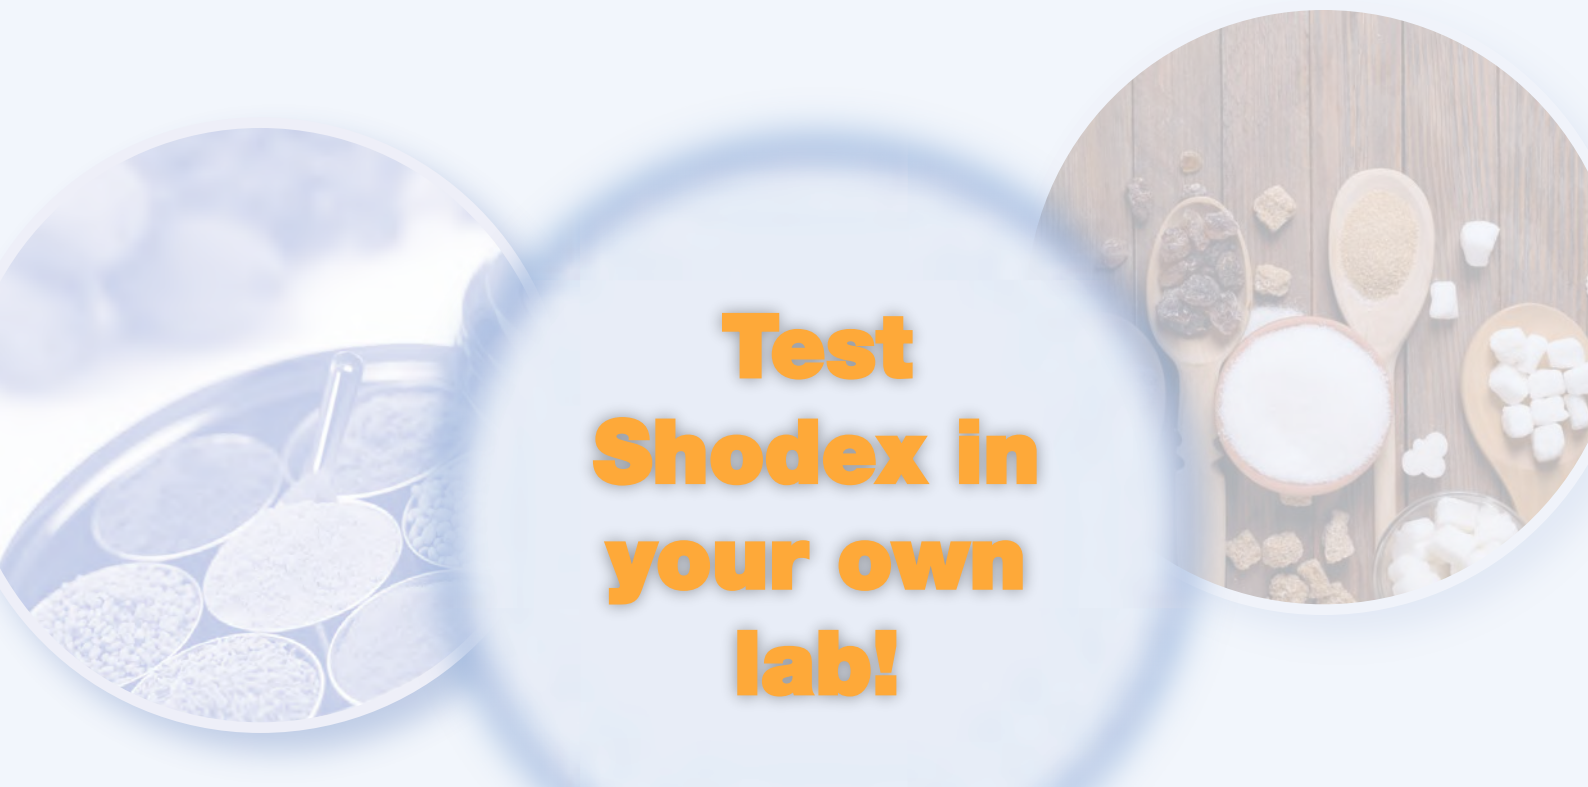

Test Shodex in your own lab!

30 days free and uncommitted trial.

Application advice from our experts.

Try your samples under your conditions in your lab!

Risk free check about the performance of our polymer-based HPLC columns.

Discussion of the test results.

You can test a Shodex column for free, just contact us!

YES



CONGRATS! YOU DID IT TO THE BEST PERFORMANCE!

YES

Are you already using them?

NO

NO

Do you know the advantages of polymer-based HPLC columns?

These are the advantages of polymer-based columns:

- The great chemical stability leads to an extended pH range (2 to 13).
- The low bleeding allows the use of sensitive detection.
- Large variety of material properties create a higher resolution.
- They are available for almost all separation techniques.
- The price per injection is cheaper than in silica-based columns due to their extended lifetime (2-3 times longer than silica-based).

Still no reason to use them?



Contents

Column selection	Types of Columns, Base Materials, Functional Groups and Ligands	2
	HPLC Separation Modes	3
	Column Selection by Sample Character and Separation Mode	3
	Column Selection (Application)	4
Analysis and preparative columns	Comparison of Shodex Reversed Phase Chromatography (RPC) Column Features	6
	Polymer-based Reversed Phase Chromatography Columns (ODP2 HP)	8
	Polymer-based Reversed Phase Chromatography Columns (Asahipak)	10
	Polymer-based Reversed Phase Chromatography Columns (RSpak)	12
Reversed Phase, Hydrophilic Interaction and Normal Phase Chromatography	Polymer-based Hydrophilic Interaction Chromatography (HILIC) Columns (HILICpak)	16
	Polymer-based Hydrophilic Interaction Chromatography (HILIC) Columns (Asahipak)	20
	Silica-based Reversed Phase Chromatography Columns (ODS Columns)	22
	Silica-based Reversed Phase Chromatography Columns (Other Columns)	22
	Silica-based Normal Phase Chromatography and HILIC Columns	23
Ligand Exchange Chromatography	Ligand Exchange Chromatography Columns	26
Ion Exclusion Chromatography	Ion Exclusion Chromatography Columns	30
Ion Chromatography	Ion Chromatography Columns (Anion Analysis)	32
	Ion Chromatography Columns (Cation Analysis)	34
	Column Selection for Size Exclusion Chromatography (SEC)	36
	Precautions for Polar Polymer Analysis	37
	Aqueous SEC (GFC) Columns: Silica-based	38
	Aqueous SEC (GFC) Columns: Polymer-based	42
	Multimode Columns	46
	Aqueous/Organic SEC Columns	48
	Organic SEC (GPC) Columns (General Analysis): THF	50
	Organic SEC (GPC) Columns (General Analysis): Chloroform	52
	Organic SEC (GPC) Columns (General Analysis): DMF	54
Size Exclusion Chromatography	Solvent-peak Separation Columns for Organic SEC (GPC)	54
	Organic SEC (GPC) Columns: Rapid Analysis	56
	Organic SEC (GPC) Columns: High Performance Analysis	56
	Organic SEC (GPC) Columns: Ultra-rapid Analysis	58
	Organic SEC (GPC) Columns: Preparative Columns	60
	Organic SEC (GPC) Columns: Linear Calibration Type	62
	Organic SEC (GPC) Columns: High Temperature/Ultra High Temperature Analysis	64
	Organic SEC (GPC) Columns: HFIP	66
	Solvent Replacement Applicability of SEC (GPC) Columns	68
	Calibration Standards for SEC	69
Ion Exchange Chromatography	Anion Exchange Chromatography Columns	70
	Cation Exchange Chromatography Columns	72
	Hydrophobic Interaction Chromatography Column	74
	Affinity Chromatography Columns	74
Special Separation Modes Columns	Chiral Separation Columns	74
	High Temperature Reversed Phase Chromatography Column	74
	Pretreatment Column for Column Switching Method	74
Sample pretreatment columns	GPC Clean-up Columns	76
Product name changes notices	Product Name Changes Notices	78
	USP40-NF35 Column List	79
	Column Cleaning Procedures	80
Information	General Precautions for Column Handling	81
	Column Trouble Shooting	82
	HPLC System Trouble Shooting	83
Index	Index by Product Name	84
	Index by Product Code	85

Types of Columns, Base Materials, Functional Groups and Ligands

Separation Type		Product Name	Base Material	Functional Group, Ligand	Page
Reversed Phase & HILIC (Polymer-based)		ODP2 HP	Polyhydroxymethacrylate	—	8
	Asahipak	ODP-50, ODP-40	Polyvinyl alcohol	Octadecyl	10
	Asahipak	C8P-50	Polyvinyl alcohol	Octyl	10
	Asahipak	C4P-50	Polyvinyl alcohol	Butyl	10
	RSpak	RP18-415, DS	Styrene divinylbenzene copolymer	—	12
	RSpak	DE	Polymethacrylate	—	12
	RSpak	DM-614	Polyhydroxymethacrylate	—	12
	RSpak	NN	Polyhydroxymethacrylate	Sulfo	12
	RSpak	JJ-50	Polyvinyl alcohol	Quaternary ammonium	12
	HILICpak	VG-50	Polyvinyl alcohol	Amino	16
	HILICpak	VT-50	Polyvinyl alcohol	Quaternary ammonium	16
	HILICpak	VC-50	Polyvinyl alcohol	Carboxyl	16
	HILICpak	VN-50	Polyvinyl alcohol	Diol	16
	Asahipak	NH2P	Polyvinyl alcohol	Amino	20
Reversed Phase, Normal Phase & HILIC (Silica-based)		ET-RP1	Polyvinyl alcohol	Octadecyl	74
		C18	Silica	Octadecyl	22
	Silica	C18M, C18P	Silica	Octadecyl	22
	Silica	5C8	Silica	Octyl	22
	Silica	5CN	Silica	Cyanopropyl	22
	Silica	5NPE	Silica	Nitrophenylethyl	22
	Silica	5PYE	Silica	Pyrenylethyl	22
	Silica	5SIL	Silica	—	23
Ligand Exchange		5NH	Silica	Aminopropyl	23
	SUGAR	SC	Styrene divinylbenzene copolymer	Sulfo (Ca ²⁺)	26
	SUGAR	SP0810	Styrene divinylbenzene copolymer	Sulfo (Pb ²⁺)	26
	SUGAR	KS-800	Styrene divinylbenzene copolymer	Sulfo (Na ⁺)	26
	RSpak	DC-613	Styrene divinylbenzene copolymer	Sulfo (Na ⁺)	26
	SUGAR	SZ5532	Styrene divinylbenzene copolymer	Sulfo (Zn ²⁺)	26
	EP	SC1011-7F	Styrene divinylbenzene copolymer	Sulfo (Ca ²⁺)	27
Ion Exclusion	USPpak	MN-431	Styrene divinylbenzene copolymer	Sulfo (Ca ²⁺)	27
	SUGAR	SH	Styrene divinylbenzene copolymer	Sulfo	30
Ion Chromatography	RSpak	KC-811	Styrene divinylbenzene copolymer	Sulfo	30
	IC	NI-424, I-524A	Polyhydroxymethacrylate	Quaternary ammonium	32
	IC	SI	Polyvinyl alcohol	Quaternary ammonium	32
	IC	YS-50	Polyvinyl alcohol	Carboxyl	34
	IC	YK-421	Silica	Carboxyl	34
Aqueous SEC (GFC)	IC	Y-521, T-521	Styrene divinylbenzene copolymer	Sulfo	34
	PROTEIN	KW-800	Silica	Hydrophilic polymer	38
	PROTEIN	LW-803	Silica	Hydrophilic polymer	38
		KW400	Silica	Hydrophilic polymer	38
	OHpak	SB-800 HQ	Polyhydroxymethacrylate	—	42
Multimode	OHpak	LB-800	Polyhydroxymethacrylate	—	42
	Asahipak	GS-HQ	Polyvinyl alcohol	—	46
Aqueous/Organic SEC	Asahipak	GF-HQ	Polyvinyl alcohol	—	48
	MSPak	GF-310	Polyvinyl alcohol	—	48
Organic SEC (GPC)	GPC	KF-800, K-800, KD-800, HK-400, HK-HFIP404, KF-600, KF-400HQ, LF, HT-800, UT-800, AT-806MS, HFIP-800, HFIP-600	Styrene divinylbenzene copolymer	—	50, 52, 54, 56, 58, 62, 64, 66
Ion Exchange	IEC	QA-825	Polyhydroxymethacrylate	Quaternary ammonium	70
	IEC	DEAE-825	Polyhydroxymethacrylate	Diethylaminoethyl	70
	IEC	DEAE3N	Polyhydroxymethacrylate	Diethylaminoethyl	70
	PIKESS	DEAE-2B	Polyhydroxymethacrylate	Diethylaminoethyl	70
	Asahipak	ES-502N	Polyvinyl alcohol	Diethylaminoethyl	70
	AXpak	WA-624	Polyhydroxymethacrylate	Diethylaminoethyl	70
	IEC	SP-825	Polyhydroxymethacrylate	Sulfopropyl	72
	IEC	SP-420N	Polyhydroxymethacrylate	Sulfopropyl	72
	IEC	SP-FT 4A	Polyhydroxymethacrylate	Sulfopropyl	72
	PIKESS	SP-2B	Polyhydroxymethacrylate	Sulfopropyl	72
	IEC	CM-825	Polyhydroxymethacrylate	Carboxymethyl	72
	Asahipak	ES-502C	Polyvinyl alcohol	Carboxymethyl	72
	CXpak	P-421S	Styrene divinylbenzene copolymer	Sulfo (Na ⁺)	72
Hydrophobic Interaction	HIC	PH-814	Polyhydroxymethacrylate	Phenyl	74
Affinity	AFpak	APA-894	Polyhydroxymethacrylate	Protein A	74
	AFpak	ACH-494	Polyhydroxymethacrylate	Choline oxydase, Acetylcholine esterase	74
Chiral Separation	ORpak	CDBS-453	Silica	β-Cyclodextrin derivative	74
	ORpak	CRX-853	Polyhydroxymethacrylate	L-Amino acid derivative	74
Column Switching Pretreatment	MSPak	GF-4A	Polyvinyl alcohol	—	74
GPC Clean-up	CLNpak	EV	Styrene divinylbenzene copolymer	—	76
	CLNpak	PAE	Polyvinyl alcohol	—	76

HPLC Separation Modes

Liquid chromatography (LC) uses liquid as mobile phase (eluent). It is an analytical method that separates a mixture of compounds based on their physical and chemical differences. High performance liquid chromatography (HPLC) is a method that introduces the mobile phase under high-pressure conditions resulting in rapid and high-performance separations. The various interactions between the analyte, stationary phase (packing material), and mobile phase are the key factors for the separation. A wide variety of separation modes can be achieved by using particular combinations of stationary and mobile phases.

Separation mode	Characteristics
Reversed Phase Chromatography (RPC)	- Separation is based on the partition equilibrium between stationary phase and mobile phase. - The polarity of the stationary phase is lower than that of the mobile phase. - Typically the mobile phase contains a mixture of organic solvents (methanol, acetonitrile, or THF) and aqueous solvents (water or buffer). - Use of lower polarity mobile phases fasten the elution.
Hydrophilic Interaction Chromatography (HILIC)	- Separation is based on hydrophilic interaction. - A high polarity stationary phase is used. - Typically the mobile phase contains a mixture of organic solvents such as acetonitrile and aqueous solvents (water or buffer). - Using the higher polarity mobile phase causes a faster elution. - Applicable for the analysis of high polar substances.
Normal Phase Chromatography (NPC)	- Separation is based on the partition equilibrium between the stationary phase and the mobile phase. - The polarity of the stationary phase is higher than that of the mobile phase. - Typically the mobile phase contains a mixture of organic solvents with different polarities such as hexane and isopropanol. - Using the higher polarity mobile phase causes a faster elution.
Ligand Exchange Chromatography (LEX)	- Separation is based on differences in analytes' coordination complex. - Stationary phase modified with metal sulfonate complex ion. - Works in combination with size exclusion or HILIC modes.
Ion Exclusion Chromatography (IEX)	- Separation is based on electrostatic interaction (repulsion) between the ion exchanger and ionic solutes. - Dissociated ionic molecules elute faster than non-dissociated forms. - Used mainly for the analysis of organic acids.
Ion Chromatography (IC)	- Separation is based on electrostatic interaction (bonding) between the ion exchanger and ionic solutes. - Electrical conductivity detector can be used with a mobile phase with low-salt concentration. - Used mainly for the analysis of inorganic compounds.
Size Exclusion Chromatography (SEC)	- Network or pores on the surface of the packing material works as molecular sieve to separate molecules based on their sizes. - To separate molecules solely based on their sizes, it requires an analytical condition without any analyte and packing gel interaction. - The bigger the molecule size, the faster the elution sequence. - Used for molecular weight or molecular distribution determination of macromolecules and qualification of oligomers.
Ion Exchange Chromatography (IEC)	- Separation is based on electrostatic interactions between the ion exchanger and ionic solutes. - The mobile phase of choice should have a sufficient buffering capacity at the pH that produces the largest charge differences between the analyte of interest. - The elution position is optimized by varying the pH, salt concentration, and/or ionic strength of the mobile phase.
Hydrophobic Interaction Chromatography (HIC)	- Separation is based on hydrophobic interaction. - Hydrophobic functional group is modified on the stationary phase. - Adsorption of analytes generally occurs at a high salt concentration and they are released by lowering the salt concentration. - Used mainly for the analysis of proteins.
Affinity Chromatography (AFC)	- Separation is based on adsorption of the analyte to the specific biologically derived ligand pair. - Highly selective. - A buffer solution with the appropriate pH and ionic strength is selected based on the type of ligand, analytes, and their interaction. - Used mainly for the purification and concentration of biologically active substances.
Chiral Separation Chromatography (CS)	- Separation of optical isomers using chiral selectors. - Highly selective.
Multimode Chromatography	Separation is based on the combination of different modes.

Column Selection by Sample Character and Separation Mode

Sample Solubility	Sample MW	Separation Mode	Sample Solubility	Sample MW	Separation Mode
Aqueous soluble	≥ 2,000	RPC	Organic soluble	≥ 2,000	SEC
		LEX			
		IEX			
		SEC			
		IEC			
		HIC			
		AFC			
	≤ 2,000	RPC		≤ 2,000	RPC
		HILIC			
		LEX			
		IEX			NPC
		IC			
		SEC			
		IEC			SEC
		AFC			
		CS			

RPC : Reversed Phase Chromatography

HILIC : Hydrophilic Interaction Chromatography

NPC : Normal Phase Chromatography

LEX : Ligand Exchange Chromatography

IEX : Ion Exclusion Chromatography

IC : Ion Chromatography

SEC : Size Exclusion Chromatography

IEC : Ion Exchange Chromatography

HIC : Hydrophobic Interaction Chromatography

AFC : Affinity Chromatography

CS : Chiral Separation Chromatography

Column Selection (Application)

Pharmaceuticals, Cosmetics

		Separation Mode	Page
Pharmaceuticals Metabolites Additives	Hydrophobic substances	RPC	8, 10, 12, 22
	Hydrophilic substances	HILIC	16, 20
		IEC+RPC	12
		LEX+SEC	26, 27
	Substances in bio-fluid (serum-plasma-urine)	RPC	8
		SEC+RPC	46, 48
	Polymer	SEC	38, 42, 48, 54, 62
Moisturizers	Polyalcohols	RPC	12
		LEX+SEC	26
		LEX+HILIC	26
		SEC	42, 48
	Protein hydrolysates	RPC	10, 12
		SEC	38
	Mucopolysaccharides	SEC	42
Emulsifiers	Surfactants	SEC+RPC	48
		SEC	50, 56, 58
Preservatives	Paraben Dehydroacetic acid	RPC	10, 12, 22
Optical active materials		CS	74

Foods

		Separation Mode	Page
Nutritional ingredients	Monosaccharides Disaccharides Sugar alcohols	HILIC	16, 20
		LEX+SEC	26
		LEX+HILIC	26
	Oligosaccharides	HILIC	16, 20
		LEX+HILIC	26
		SEC	26, 42, 46
	Low molecular weight water-soluble dietary fiber	SEC	46
	Polysaccharides	SEC	26, 42
	Organic acids	RPC	8, 12
		IEC+RPC	30
		IC	32
	Water-soluble vitamins	RPC	8, 10, 12
		IEC+RPC	12
		HILIC	16, 20
	Fat-soluble vitamins	RPC	10
		NPC	23
		SEC	50, 54
	Fatty acids	RPC	12, 22
		SEC	48, 50, 52, 54
Food safety	Food additives	IEC+SEC	46
		IEC+IEC+RPC	12
	Pesticides	HILIC	16
		IC	34
		IEC	72
		SEC	76
	Mycotoxin	RPC	22
		SEC	76
	Pretreatment of residual pesticides	SEC	76
		GPC (clean-up)	76
	Organic solvent soluble	RPC	10, 12, 74
		HILIC	16, 20
		RPC	12
		IEC+RPC	12
	Polar organic solvent soluble	HILIC	16
		IC	32
	High temperature/ Ultra high temperature	RPC	22
		SEC	76
	Water-soluble	SEC	76

Separation Mode (Page 4 and Page 5)

RPC : Reversed Phase Chromatography
 HILIC : Hydrophilic Interaction Chromatography
 NPC : Normal Phase Chromatography
 LEX : Ligand Exchange Chromatography
 IEX : Ion Exclusion Chromatography
 IC : Ion Chromatography
 SEC : Size Exclusion Chromatography
 IEC : Ion Exchange Chromatography
 HIC : Hydrophobic Interaction Chromatography
 AFC : Affinity Chromatography
 CS : Chiral Separation Chromatography

New Materials

		Separation Mode	Page
Synthetic polymers	Organic solvent soluble	SEC	48, 50, 52, 54, 56, 58
	Polar organic solvent soluble		42, 48, 54, 56, 58, 62
	High temperature/ Ultra high temperature		64
	Water-soluble		38, 42, 46, 48
Additives Oligomers		RPC	10, 12, 22
	Organic solvent soluble	SEC	48, 50, 52, 56, 58
	Polar organic solvent soluble		42, 48, 54, 56, 58
	Water-soluble		38, 42, 46, 48

Biotechnology

		Separation Mode	Page
Genomics	Nucleobases Nucleotides Nucleosides	RPC	12
		IEC+SEC	12, 46
		IEC	70
	Oligo nucleic acids	HILIC	16
		RPC	12
		IEC+SEC	46
		IEC	70
	DNA/RNA	SEC	42, 46
Proteomics	Amino acids	RPC	10
		IEC+IEX+RPC	12
		HILIC	16
		IEC	72
		IEC+SEC	46
	Peptides Proteins	RPC	10, 12
		SEC	38, 42, 46, 48
		IEC	70, 72
		HIC	74
Glycomics	Glycoproteins	RPC	10, 12
		SEC	38, 42, 46, 48
		IEC	70, 72
		HIC	74
	Sugar chains	HILIC	16, 20
	Monosaccharides	HILIC	16, 20
		LEX+SEC	26
		LEX+HILIC	26
	Sialic acids Uronic acids Aldonic acids	IEX+RPC	30
Hormones	Amines	RPC	8, 10, 12
		IEC	72
	Steroids	RPC	10
		HILIC	16, 20
		SEC	42, 48
Lipids	Phospholipids	NPC	23
		SEC	48, 50, 54
	Lipoproteins	SEC	38, 42

Environment

		Separation Mode	Page
Water quality	Anions	IC	32
	Oxyhalides	IC	32
		IEC+HILIC	16
	Cyanide Cyanogen chloride	IEX	30
	Cations	IC	34
	Surfactants	RPC	10, 22
		SEC+RPC	48
	Pesticides	RPC	12, 22
		IEC+RPC	12
		HILIC	16
		IC	32
Soil	Anions	IC	32
	Heavy metals	IC	34
	Humic substances	SEC	42
	Organic arsenic	IEX+RPC	12
	Pesticides	RPC	12, 22
		IEC+RPC	12
		HILIC	16
		IC	32
Environmental hormones	Pretreatment of Phthalates PCBs Benzo [a] pyrene	SEC GPC (clean-up)	76
Bioethanols	Monosaccharides Oligosaccharides	HILIC	16, 20
		LEX+SEC	26
	Oligosaccharides Alcohols Furfural	LEX+SEC	26
	Saccharides Organic acids Alcohols Furfural	IEX+RPC+SEC	30
	Hemicelluloses Celluloses	SEC	54, 62
Biodiesels	Cations	IC	34
	Fatty acid glycerides	SEC	48
	Fatty acid methyl esters	RPC	12
	Organic acids	IC	32


● Comparison of Shodex Reversed Phase Chromatography (RPC) Column Features

ODS columns are the most popular reversed phase columns that are packed with silica-based octadecyl group. Shodex provides not only ODS columns but also polymer-based reversed phase columns with different functional groups. Please use following descriptions about the column features as guidelines to select suitable columns for your application purposes.


Features

ODP2 HP	- Provides a large theoretical plate number nearly twice as much as generally available polymer-based reversed phase columns do - Offers enhanced retention of high polar substances compared to ODS columns - Suitable for the analysis of small molecules such as pharmaceuticals in the presence of protein matrix - Ideal for LC/MS analysis of high polar compounds - Fulfills USP L39 requirements
ODP-50	Relatively large pore size is suitable for the analysis of amino acids, peptides, and proteins
C8P-50	Usable in a wide pH range from pH 2 to 13
C4P-50	- Usable in 100% water and buffer solution - Best used for the analysis of basic substances - ODP-50 fulfills USP L67 requirements
ODP-40	- Higher performance type of ODP-50 series - Fulfills USP L67 requirements
RP18-415	- Large pore size is suitable for the analysis of proteins and peptides - Fulfills USP L21 requirements
DS-613	Suitable for reversed phase analysis of highly hydrophilic substances that are not well retained by ODS columns
DS-413	Fulfill USP L21 requirements
DE	- General purpose polymer-based column having similar polarity as ODS columns - Wide working pH range (from pH 2 to 12), usable in 100% water and buffer solutions - Fulfills USP L71 requirements
DM-614	- Suitable for the analysis of amino acids and water-soluble vitamins - Fulfills USP L39 requirements
NN	- The packing material modified with sulfo groups supports multimode (reversed phase and cation exchange) analysis - Ideal for the analysis of complex samples containing neutral and ionic substances
JJ-50	- The packing material is modified with trace amounts of quaternary ammonium groups, and supports multimode (reversed phase and anion exchange) analysis - Ideal for analysis of complex samples containing neutral and ionic substances
C18	- Fully end capped ODS column available at very reasonable price - Fulfills USP L1 requirements
C18M	- Monomeric type ODS column fully end capped high purity silica (99.99% or higher) - Fulfills USP L1 requirements
C18P	- Polymeric type ODS column fully end capped high purity silica (99.99% or higher) - Excellent acid tolerance - Advantageous for separating planar and nonplanar compounds from each other - Fulfills USP L1 requirements
5C8	- Use when the retention capacity of C18 is too strong - Rapid mass transfer and fast equilibration allow its use as an ion-pair chromatography - Fulfills USP L7 requirements
5CN	- Utilizes reversed phase interaction and π-electron interaction to separate regioisomers, which typically cannot be separated with ODS or C8 columns - Fulfills USP L10 requirements
5NPE	Utilizes several types of interactions based on π-electrons to separate structural isomers
5PYE	5NPE fulfills USP L11 requirements

The interrelation between hydrophobicity and retention, and the interrelation between steric selectivity and retention were compared among Shodex columns for reversed phase chromatography. The retention factor (k') of amylbenzene was used as the retention, the separation factor (α) between n-butylbenzene and n-amylbenzene was used as the hydrophobicity. The separation factor between o-terphenyl and triphenylene was used as the steric recognition. Larger separation factor means higher hydrophobicity and higher steric selectivity.

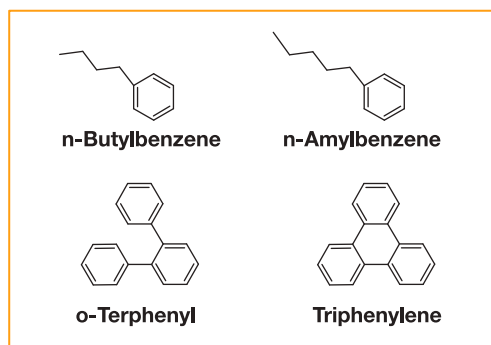


Hydrophobicity differences among Shodex RPCs

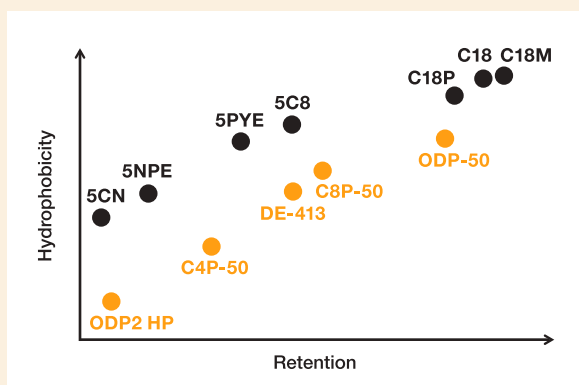


Column size : 4.6mm I.D. x 150mm each
 Eluent : H₂O/CH₃OH=20/80
 Flow rate : 1.0mL/min
 Detector : UV (254nm)
 Column temp. : 40°C

Steric selectivity differences among Shodex RPCs

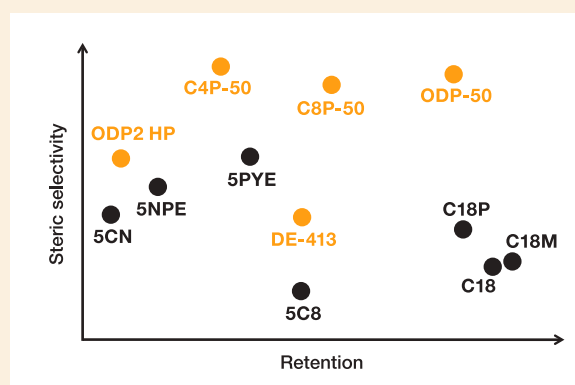


Column size : 4.6mm I.D. x 150mm each
 Eluent : H₂O/CH₃OH=20/80
 Flow rate : 1.0mL/min
 Detector : UV (254nm)
 Column temp. : 40°C

Comparison of different functional groups on the separation of alkylalcohols

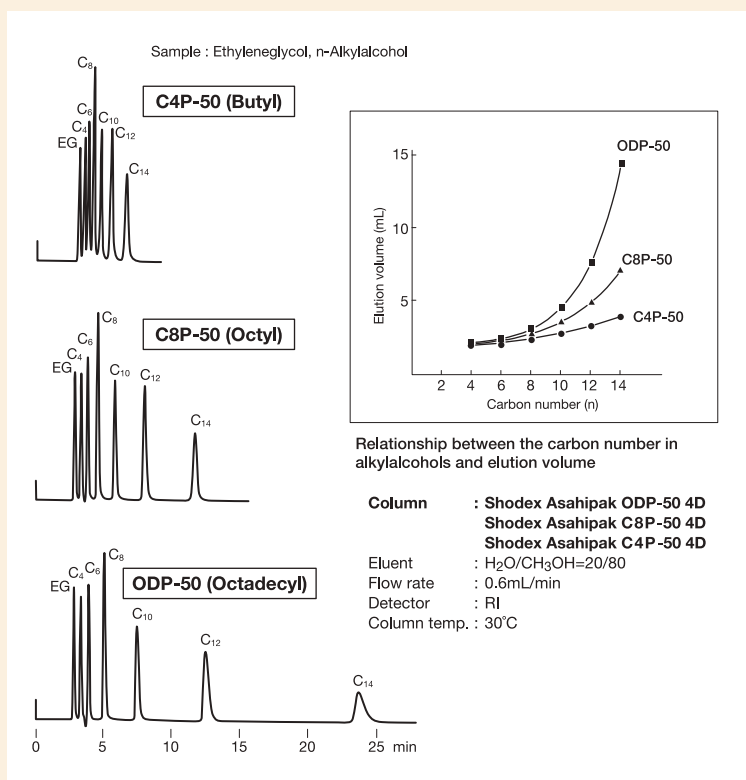

Effects of steric selectivity differences

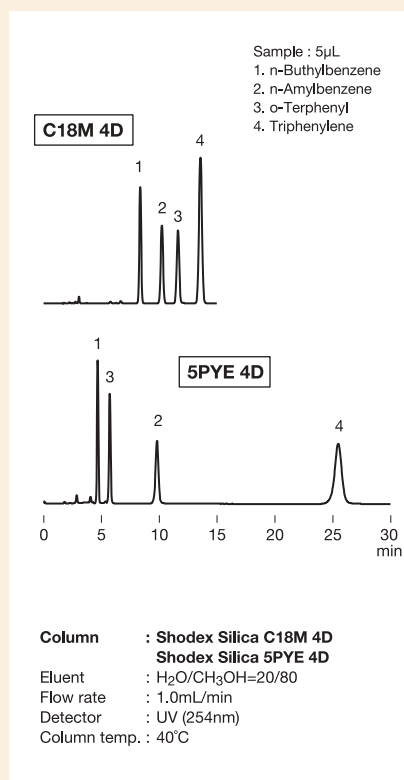

Polymer-based Reversed Phase Chromatography Columns (ODP2 HP)

Please refer to “Comparison of Shodex Reversed Phase Chromatography (RPC) Column Features” on page 6 and 7 for features.

Standard columns

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7622001	ODP2 HP-4B	≥ 3,500	–	5	40	4.6 × 50	H ₂ O/CH ₃ CN=55/45
F7622002	ODP2 HP-4D	≥ 13,000	–	5	40	4.6 × 150	H ₂ O/CH ₃ CN=55/45
F7622003	ODP2 HP-4E	≥ 17,000	–	5	40	4.6 × 250	H ₂ O/CH ₃ CN=55/45
F6714010	ODP2 HPG-4A	(guard column)	–	5	–	4.6 × 10	H ₂ O/CH ₃ CN=55/45
F7622004	ODP2 HP-2B	≥ 3,000	–	5	40	2.0 × 50	H ₂ O/CH ₃ CN=55/45
F7622005	ODP2 HP-2D	≥ 7,000	–	5	40	2.0 × 150	H ₂ O/CH ₃ CN=55/45
F6714011	ODP2 HPG-2A	(guard column)	–	5	–	2.0 × 10	H ₂ O/CH ₃ CN=55/45

Base Material: Polyhydroxymethacrylate

3mm I.D columns [Customized columns]

Product Code	Product Name	Functional Group	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F7622006	ODP2 HP-3B	–	5	40	3.0 × 50
F7622007	ODP2 HP-3D	–	5	40	3.0 × 150
F6714014	ODP2 HPG-3A (guard column)	–	5	–	3.0 × 10


Base Material: Polyhydroxymethacrylate

Preparative columns *Preparative columns are made to order.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6822001	ODP2 HP-10E	≥ 9,500	6	10.0 × 250	ODP2 HP
F6714015	ODP2 HPG-7B	(guard column)	6	7.5 × 50	(guard column)

Comparison between ODP2 HP-4D and ODS column for their alkaline tolerances


Chromatograms obtained before and after passing alkaline eluent

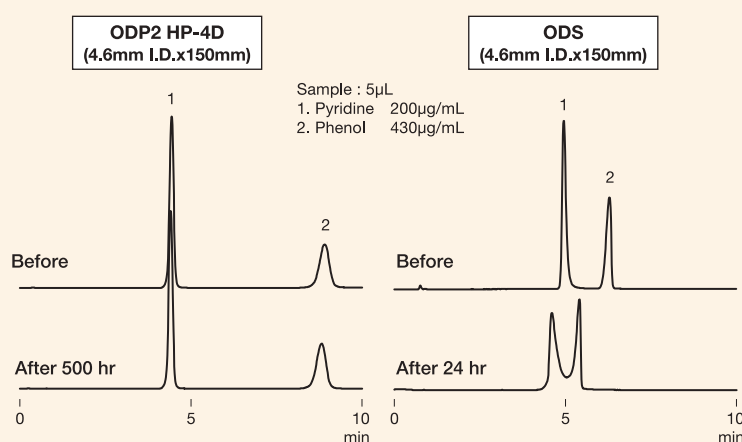

Analysis condition

Column : Shodex ODP2 HP-4D
 ODS from other manufacturer
 Eluent : H₂O/CH₃OH=70/30
 Flow rate : 1.0mL/min
 Detector : UV (254nm)
 Column temp. : 40°C

Correlation between alkaline eluent passing time and relative theoretical plate number

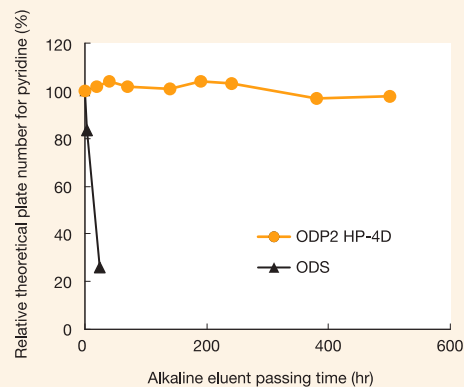


Eluent passing conditions for alkali tolerance test

Column : Shodex ODP2 HP-4D
 ODS from other manufacturer
 Eluent : 10mM Sodium phosphate buffer (pH12)
 /CH₃CN=45/55
 Flow rate : 0.6mL/min
 Column temp. : 30°C

Comparison between ODP2 HP and ODP-50 (existing)

Sample : 5 μ L
 1. Phenol 300mg/L
 2. Methyl benzoate 350mg/L
 3. Toluene 1000mg/L
 4. Naphthalene 150mg/L

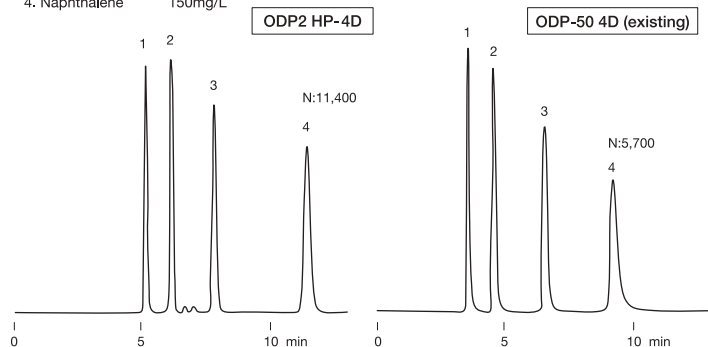


Column : Shodex ODP2 HP-4D
Eluent : H₂O/CH₃CN=55/45
Flow rate : 0.6mL/min
Detector : UV (254nm)
Column temp. : 40°C

Column : Shodex Asahipak ODP-50 4D
Eluent : H₂O/CH₃CN=35/65
Flow rate : 0.6mL/min
Detector : UV (254nm)
Column temp. : 40°C

Imidazoles


Sample : 0.1% each, 10 μ L
 1. Imidazole
 2. 2-Methylimidazole
 3. 4-Methylimidazole

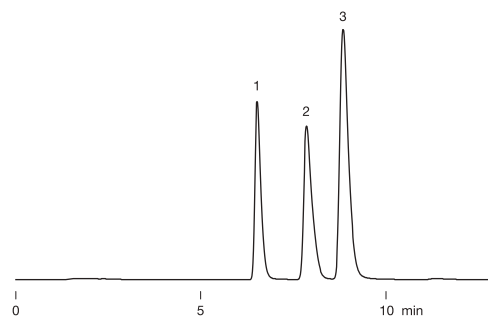

Column : Shodex ODP2 HP-4E
Eluent : 10mM Na₂HPO₄ aq./CH₃CN=90/10
Flow rate : 0.8mL/min
Detector : UV (220nm)
Column temp. : 40°C


Influence of repeated protein injection on column pressure

ODP2 HP columns are packed with gels with increased surface polarity and smaller pore size which prevent the adsorption of proteins. BSA was injected multiple times to both ODS and ODP2 HP columns. A significant column pressure increase was observed for the ODS column, while no considerable change was observed for the ODP2 HP column even after 140 injections.

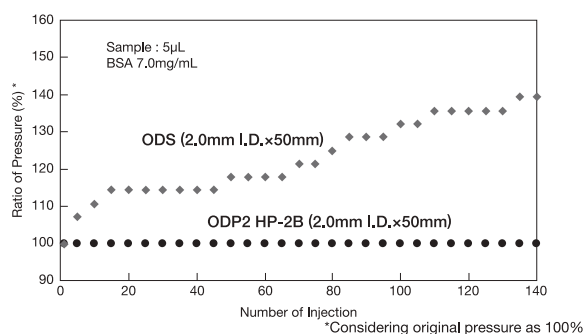

Column : Shodex ODP2 HP-2B
ODS from other manufacturer
Eluent : 1mM CH₃COONH₄ aq./CH₃CN=90/10
Flow rate : 0.2mL/min
Detector : UV (220nm)
Column temp. : 30°C

Anticonvulsant in serum

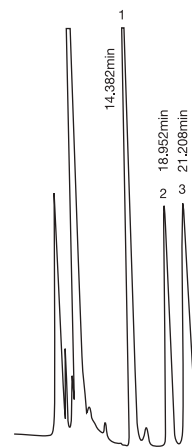



Sample : 20 μ L
 1. 2-Acetaminophenol (I.S.) 10 μ g/mL
 2. Zonisamide 13.0 μ g/mL
 3. Phenobarbital 19.0 μ g/mL
 4. Carbamazepine 4.5 μ g/mL
 5. Phenytoin 9.0 μ g/mL

Sample pretreatment:
 Mix the same volumes of serum and acetonitrile. Centrifuge the mixture at 6000g for 5 minutes. Use the supernatant as sample.

Data courtesy of Katsuko Hara.MT
 Yutaka Komiya.M.D.,
 Department of Clinical Sciences
 and Laboratory Medicine,
 Kansai Medical University.

Column : Shodex ODP2 HP-4E
Eluent : 25mM Sodium phosphate buffer (pH5.2)/CH₃CN=680/320
Flow rate : 0.35mL/min
Detector : UV (210nm)
Column temp. : 40°C

Comparison of barbital recovery rate using ODP2 HP-2B and ODS in the presence of BSA

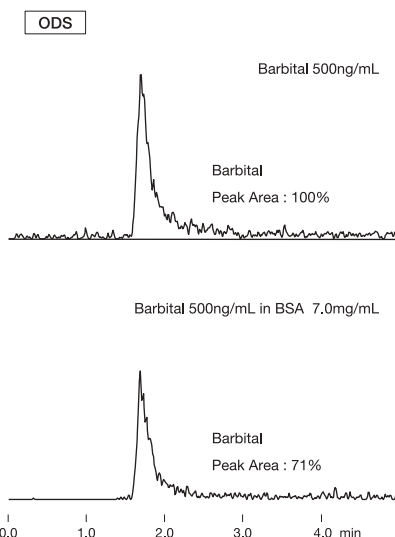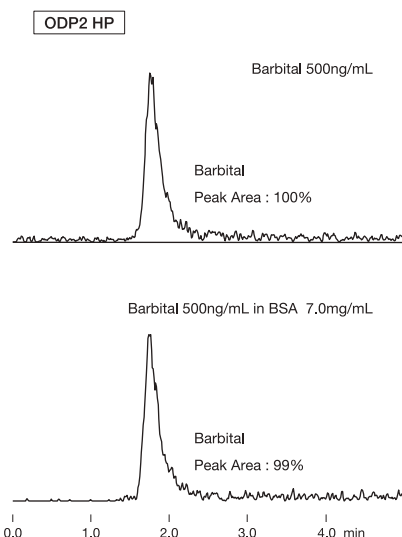

For the LC/MS analysis of drugs in samples containing protein matrix, use of ODP2 HP column showed less matrix effect (ion suppression in this case) compared to when ODS column was used. This shows that ODP2 HP column does not retain protein and elute it as a void.

Column : Shodex ODP2 HP-2B
ODS from other manufacturer
Eluent : 10mM Ammonium acetate aq./CH₃CN=70/30
Flow rate : 0.2mL/min
Detector : ESI-MS (SIM Negative : m/z 183)
Column temp. : 30°C
Injection vol. : 10 μ L

Polymer-based Reversed Phase Chromatography Columns (Asahipak)

Please refer to “Comparison of Shodex Reversed Phase Chromatography (RPC) Column Features” on page 6 and 7 for features.

Standard columns

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7621001	Asahipak ODP-40 4D	≥ 11,000	Octadecyl	4	250	4.6 × 150	H ₂ O/CH ₃ CN=35/65
F7621002	Asahipak ODP-40 4E	≥ 17,000	Octadecyl	4	250	4.6 × 250	H ₂ O/CH ₃ CN=35/65
F7620002	Asahipak ODP-50 6D	≥ 9,000	Octadecyl	5	250	6.0 × 150	H ₂ O/CH ₃ CN=35/65
F7620001	Asahipak ODP-50 6E	≥ 14,000	Octadecyl	5	250	6.0 × 250	H ₂ O/CH ₃ CN=35/65
F6710001	Asahipak ODP-50G 6A	(guard column)	Octadecyl	5	–	6.0 × 10	H ₂ O/CH ₃ CN=35/65
F6710023	Asahipak ODP-50 4B	≥ 2,500	Octadecyl	5	250	4.6 × 50	H ₂ O/CH ₃ CN=35/65
F7620004	Asahipak ODP-50 4D	≥ 9,000	Octadecyl	5	250	4.6 × 150	H ₂ O/CH ₃ CN=35/65
F7620003	Asahipak ODP-50 4E	≥ 14,000	Octadecyl	5	250	4.6 × 250	H ₂ O/CH ₃ CN=35/65
F6710022	Asahipak ODP-50G 4A	(guard column)	Octadecyl	5	–	4.6 × 10	H ₂ O/CH ₃ CN=35/65
F7620009	Asahipak ODP-50 2D	≥ 5,000	Octadecyl	5	250	2.0 × 150	H ₂ O/CH ₃ CN=35/65
F6713001	Asahipak ODP-50G 2A	(guard column)	Octadecyl	5	–	2.0 × 10	H ₂ O/CH ₃ CN=35/65
F7620006	Asahipak C8P-50 4D	≥ 7,000	Octyl	5	250	4.6 × 150	H ₂ O/CH ₃ CN=35/65
F7620005	Asahipak C8P-50 4E	≥ 11,000	Octyl	5	250	4.6 × 250	H ₂ O/CH ₃ CN=35/65
F6710002	Asahipak C8P-50G 4A	(guard column)	Octyl	5	–	4.6 × 10	H ₂ O/CH ₃ CN=35/65
F7620008	Asahipak C4P-50 4D	≥ 6,000	Butyl	5	250	4.6 × 150	H ₂ O/CH ₃ CN=35/65
F7620007	Asahipak C4P-50 4E	≥ 9,000	Butyl	5	250	4.6 × 250	H ₂ O/CH ₃ CN=35/65
F6710003	Asahipak C4P-50G 4A	(guard column)	Butyl	5	–	4.6 × 10	H ₂ O/CH ₃ CN=35/65

Base Material: Polyvinyl alcohol

3mm I.D columns [Customized columns]

Product Code	Product Name	Functional Group	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F7621101	Asahipak ODP-40 3B	Octadecyl	4	250	3.0 × 50
F7621102	Asahipak ODP-40 3D	Octadecyl	4	250	3.0 × 150
F6714013	Asahipak ODP-40G 3A (guard column)	Octadecyl	4	250	3.0 × 10

Base Material: Polyvinyl alcohol

Semi-micro columns *The following semi-micro columns are made to order.


Product Code	Product Name	Functional Group	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F7838023	ODP40-2B	Octadecyl	4	250	2.0 × 50
F7838022	ODP40-2D	Octadecyl	4	250	2.0 × 150

Base Material: Polyvinyl alcohol

Preparative columns *Preparative columns are made to order.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6820001	Asahipak ODP-50 10E	≥ 10,000	5	10.0 × 250	ODP-40, ODP-50
F6820035	Asahipak ODP-90 20F	≥ 9,000	9	20.0 × 300	ODP-40, ODP-50
F6710004	Asahipak ODP-130G 7B	(guard column)	13	7.5 × 50	(guard column)
F6820003	Asahipak C8P-50 10E	≥ 8,000	5	10.0 × 250	C8P-50
F6714004	Asahipak C8P-50G 7B	(guard column)	5	7.5 × 50	(guard column)
F6820005	Asahipak C4P-50 10E	≥ 7,000	5	10.0 × 250	C4P-50
F6714005	Asahipak C4P-50G 7B	(guard column)	5	7.5 × 50	(guard column)


Alkaline tolerance of ODP-50

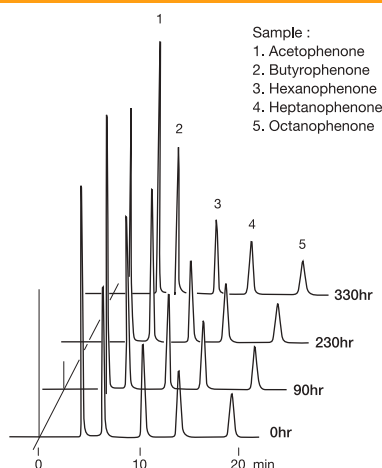

Column : Shodex Asahipak ODP-50 4D
Eluent : 10mM NaOH aq. (pH12.0)/CH₃CN=35/65
Flow rate : 0.6mL/min
Detector : UV (254nm)
Column temp. : 30°C


Local anesthetics

Dissociation of tertiary amino groups in basic drugs can be suppressed by making pH of the eluent higher than pKa of the amino groups. This increases the relative hydrophobicity of the basic drugs, thereby allowing the column to retain the drugs stronger and provide baseline separation of them.

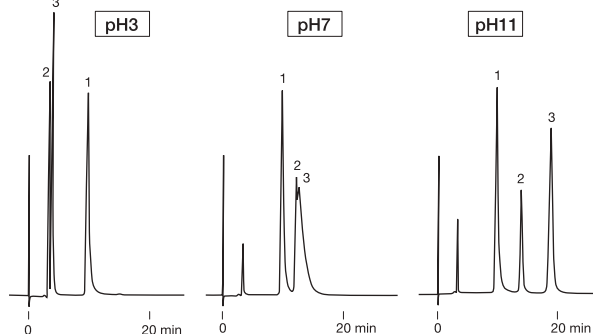


Column : Shodex Asahipak ODP-50 4D
Eluent : 25mM Phosphate buffer/CH₃CN=60/40
Flow rate : 0.6mL/min
Detector : UV (254nm)
Column temp. : 30°C

LC/MS analysis of basic drugs

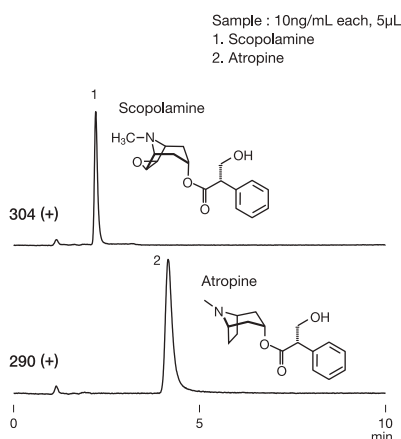


Column : Shodex ODP40-2D
Eluent : 0.05% NH₃ aq./CH₃CN=50/50
Flow rate : 0.2mL/min
Detector : ESI-MS (SIM)
Column temp. : 30°C

Fat-soluble vitamins

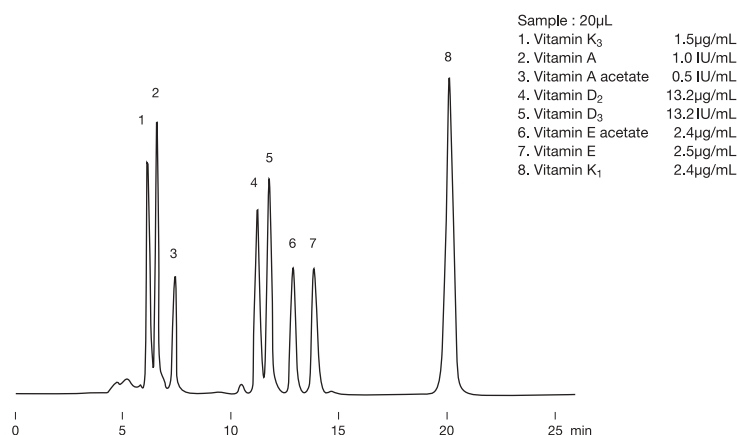


Column : Shodex Asahipak ODP-50 4E
Eluent : CH₃CN/CH₃OH=50/50
Flow rate : 0.6mL/min
Detector : UV (280nm)
Column temp. : 30°C

Analysis of azithromycin following USP method

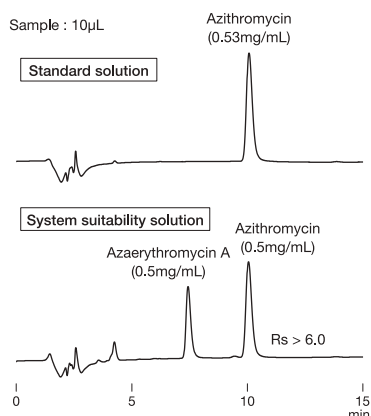


Column : Shodex Asahipak ODP-50 4E
Eluent : 6.7g/L Dibasic potassium phosphate aq. (pH11.0 adjusted with 10M KOH) /CH₃CN=40/60
Flow rate : 1.0mL/min
Detector : UV (210nm)
Column temp. : 40°C

Unsaturated fatty acids

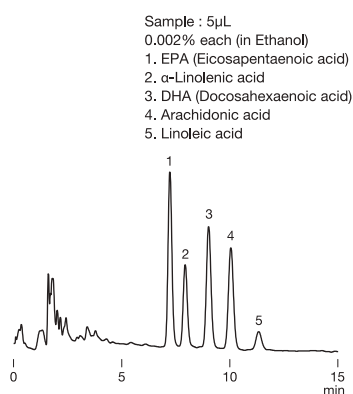

Column : Shodex Asahipak ODP-50 4D
Eluent : 0.1% H₃PO₄ in (H₂O/CH₃CN=30/70)
Flow rate : 1.0mL/min
Detector : UV (215nm)
Column temp. : 40°C

Gradient analysis of proteins and peptides

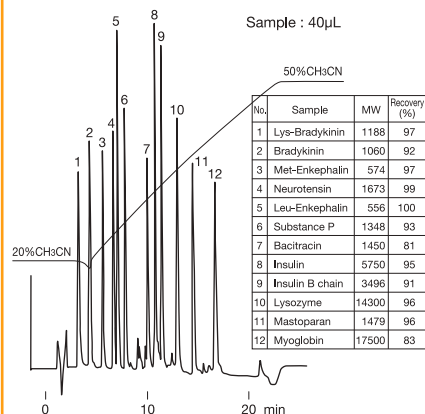

Column : Shodex Asahipak ODP-50 6D
Eluent : (A); 0.05% TFA aq./CH₃CN=80/20
 (B); 0.05% TFA aq./CH₃CN=50/50
 Linear gradient; (A) to (B), 20min
Flow rate : 1.0mL/min
Detector : UV (220nm)
Column temp. : 30°C

Polymer-based Reversed Phase Chromatography Columns (RSpak)

Please refer to “Comparison of Shodex Reversed Phase Chromatography (RPC) Column Features” on page 6 and 7 for features.

Standard columns

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Base Material	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7009000	RSpak RP18-415	≥ 5,000	–	Styrene divinylbenzene copolymer	6	450	4.6 × 150	H ₂ O/CH ₃ CN=5/95
F6709558	RSpak RP18-G	(guard column)	–	Styrene divinylbenzene copolymer	6	–	4.6 × 10	H ₂ O/CH ₃ CN/THF=40/30/30
F7001001	RSpak DS-613	≥ 6,500	–	Styrene divinylbenzene copolymer	6	200	6.0 × 150	H ₂ O/CH ₃ CN/THF=30/40/30
F7001012	RSpak DS-413	≥ 11,000	–	Styrene divinylbenzene copolymer	3.5	200	4.6 × 150	H ₂ O/CH ₃ CN/THF=40/30/30
F6700140	RSpak DS-G	(guard column)	–	Styrene divinylbenzene copolymer	10	–	4.6 × 10	H ₂ O/CH ₃ CN/THF=30/40/30
F7001004	RSpak DE-613	≥ 7,000	–	Polymethacrylate	6	25	6.0 × 150	H ₂ O
F7001005	RSpak DE-413	≥ 11,000	–	Polymethacrylate	4	25	4.6 × 150	H ₂ O/CH ₃ CN=50/50
F7009030	RSpak DE-413L	≥ 17,000	–	Polymethacrylate	4	25	4.6 × 250	H ₂ O/CH ₃ CN=50/50
F6700150	RSpak DE-G 4A (RSpak DE-G)	(guard column)	–	Polymethacrylate	10	–	4.6 × 10	H ₂ O
F7001007	RSpak DE-213	≥ 8,000	–	Polymethacrylate	4	25	2.0 × 150	H ₂ O/CH ₃ CN=50/50
F6700151	RSpak DE-G 2A (RSpak DE-SG)	(guard column)	–	Polymethacrylate	6	–	2.0 × 10	H ₂ O/CH ₃ CN=50/50
F7001002	RSpak DM-614	≥ 4,500	–	Polyhydroxymethacrylate	10	200	6.0 × 150	5mM H ₃ PO ₄ aq.
F6700160	RSpak DM-G 4A (RSpak DM-G)	(guard column)	–	Polyhydroxymethacrylate	12	–	4.6 × 10	5mM H ₃ PO ₄ aq.
F7008140	RSpak NN-814	≥ 9,000	Sulfo	Polyhydroxymethacrylate	10	200	8.0 × 250	0.1M Sodium phosphate buffer (pH3.0)
F7008150	RSpak NN-614	≥ 4,000	Sulfo	Polyhydroxymethacrylate	10	200	6.0 × 150	0.1M Sodium phosphate buffer (pH3.0)
F6700510	RSpak NN-G	(guard column)	Sulfo	Polyhydroxymethacrylate	10	–	6.0 × 50	0.1M Sodium phosphate buffer (pH3.0)
F7008160	RSpak NN-414	≥ 6,000	Sulfo	Polyhydroxymethacrylate	10	200	4.6 × 150	0.1M Sodium phosphate buffer (pH3.0)
F7008240	RSpak JJ-50 4D	≥ 4,500	Quaternary ammonium	Polyvinyl alcohol	5	100	4.6 × 150	H ₂ O/CH ₃ CN=40/60
F7008220	RSpak JJ-50 2D	≥ 3,500	Quaternary ammonium	Polyvinyl alcohol	5	100	2.0 × 150	H ₂ O/CH ₃ CN=40/60


■ **Semi-micro columns** *The following semi-micro columns are made to order.

Product Code	Product Name	Functional Group	Base Material	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F7840123	DE413-2B	–	Polymethacrylate	4	25	2.0 × 50
F7840121	DE413-2E	–	Polymethacrylate	4	25	2.0 × 250
F7860122	NN414-2D	Sulfo	Polyhydroxymethacrylate	10	200	2.0 × 150

■ **Preparative columns** *Preparative columns are made to order.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6513013	RSpak DE-2013	≥ 10,000	12	20.0 × 300	DE-413, DE-613
F6700190	RSpak DE-G 8B (RSpak DE-LG)	(guard column)	12	8.0 × 50	DE-413, DE-613
F6514014	RSpak DM-2014	≥ 5,000	12	20.0 × 300	DM-614
F6700404	RSpak DM-G 8B (RSpak DM-LG)	(guard column)	12	8.0 × 50	(guard column)


Separation and recovery rate of standard proteins

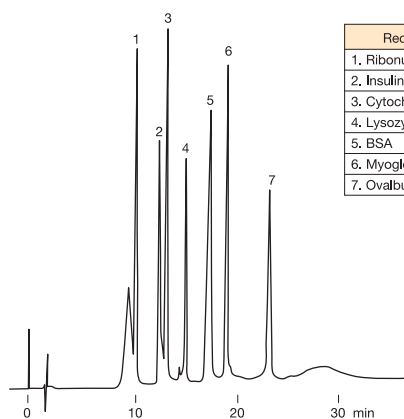

Recovery (%)	
1. Ribonuclease A	93
2. Insulin	98
3. Cytochrome c	100
4. Lysozyme	100
5. BSA	98
6. Myoglobin	108
7. Ovalbumin	—

Column : Shodex RSpak RP18-415
Eluent : (A); 0.1% TFA aq./CH₃CN=99/1
 (B); 0.1% TFA aq./CH₃CN=5/95
 Linear gradient; (B%) 20% to 60%, 20min
Flow rate : 1.0mL/min
Detector : UV (220nm)
Column temp. : Room temp.


Alkylbenzenes

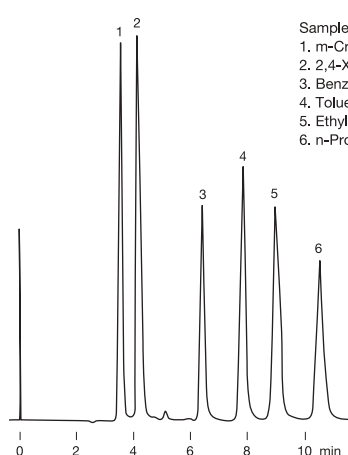

Sample : 5μL
 1. m-Cresol 0.1%
 2. 2,4-Xylenol 0.1%
 3. Benzene 0.5%
 4. Toluene 0.5%
 5. Ethylbenzene 0.5%
 6. n-Propylbenzene 0.5%

Column : Shodex RSpak DS-613
Eluent : H₂O/CH₃CN/THF=30/40/30
Flow rate : 1.0mL/min
Detector : UV (254nm)
Column temp. : 40°C


Fatty acid methyl esters

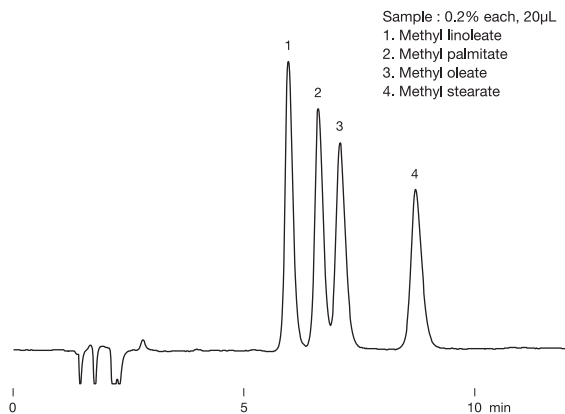

Sample : 0.2% each, 20μL
 1. Methyl linoleate
 2. Methyl palmitate
 3. Methyl oleate
 4. Methyl stearate

Column : Shodex RSpak DS-413
Eluent : H₂O/CH₃CN/THF=25/45/30
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C


Organic acids

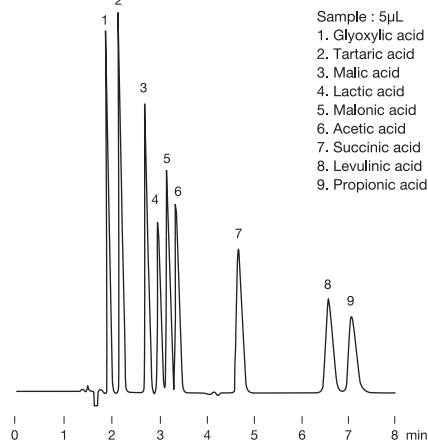

Sample : 5μL
 1. Glyoxylic acid 1.78mg/mL
 2. Tartaric acid 1.95mg/mL
 3. Malic acid 2.06mg/mL
 4. Lactic acid 2μL/mL
 5. Malonic acid 1.95mg/mL
 6. Acetic acid 2μL/mL
 7. Succinic acid 2.05mg/mL
 8. Levulinic acid 1.95mg/mL
 9. Propionic acid 2μL/mL

Column : Shodex RSpak DE-413
Eluent : 10mM H₃PO₄ aq.
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 50°C


Food additives (Preservatives)

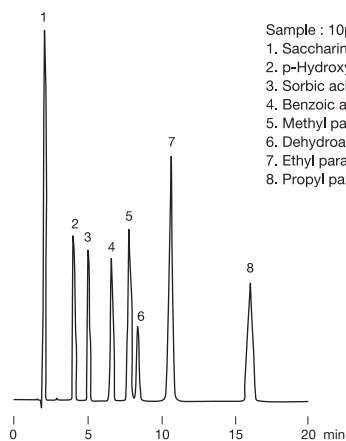

Sample : 10μL
 1. Saccharin sodium 0.005%
 2. p-Hydroxybenzoic acid 0.005%
 3. Sorbic acid 0.02%
 4. Benzoic acid 0.02%
 5. Methyl paraben 0.01%
 6. Dehydroacetic acid 0.01%
 7. Ethyl paraben 0.02%
 8. Propyl paraben 0.02%

Column : Shodex RSpak DE-413
Eluent : 50mM KH₂PO₄ + 0.1% H₃PO₄ aq.
 /CH₃CN=65/35
Flow rate : 1.0mL/min
Detector : UV (210nm)
Column temp. : 40°C


Diols

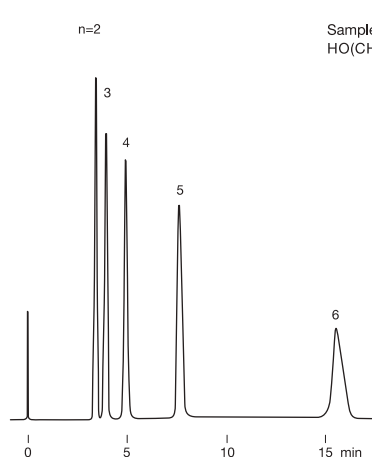

Sample : 1% each, 7.5μL
 HO(CH₂)_nOH

Column : Shodex RSpak DE-613
Eluent : H₂O
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 60°C

LC/MS analysis of organic acids

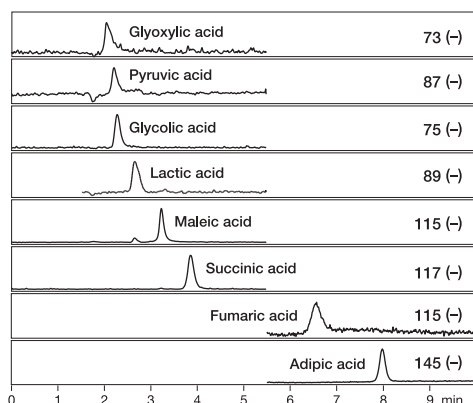


Sample : 50ng/mL each, 10μL

Column : Shodex RSpak DE-213
Eluent : (A); 0.1% (v/v) Formic acid aq./ (B); CH₃CN
 Linear gradient; (B%) 5% (0min) → 5% (2min) → 15% (2.5min) → 15% (10min)
Flow rate : 0.2mL/min
Detector : ESI-MS (SIM)
Column temp. : 30°C


Carnitine

Sample : 20μL
 1. L-Carnitine 0.1%

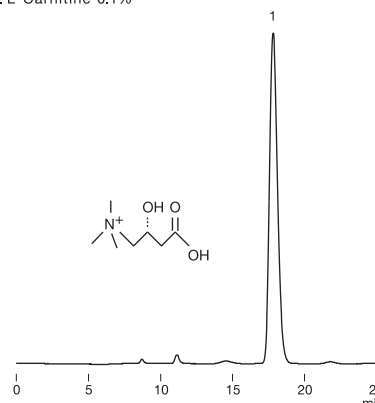

Column : Shodex RSpak NN-814
Eluent : 0.1M H₃PO₄ aq.
Flow rate : 1.0mL/min
Detector : UV (210nm)
Column temp. : 25°C


Amino acids

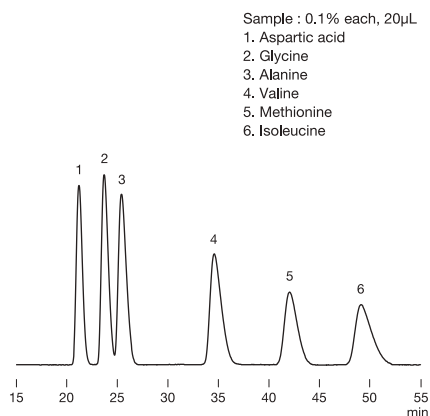


Sample : 0.1% each, 20μL
 1. Aspartic acid
 2. Glycine
 3. Alanine
 4. Valine
 5. Methionine
 6. Isoleucine

Column : Shodex RSpak NN-814
Eluent : 40mM H₃PO₄ aq.
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C


Speciation of arsenic

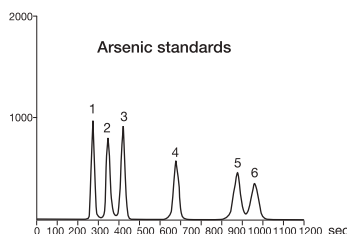

Sample : Arsenic standards, 50μL
 1. Monomethylarsonic acid
 2. Arsinic acid
 3. Dimethylarsinic acid
 4. Arsenobetaine
 5. Tetramethylarsonium
 6. Trimethylarsine oxide

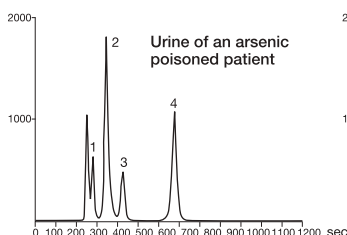


Column : Shodex RSpak NN-614
Eluent : 5mM HNO₃/8mM NH₄NO₃ aq.
Flow rate : 0.8mL/min
Detector : ICP-MS (SIM m/z 75)

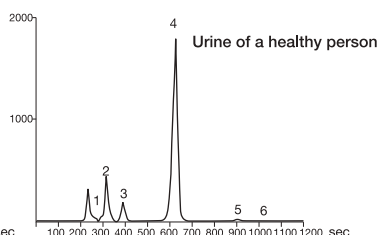

Source :
 Noriko Tsunoda,
 Pharmacia. 1998, vol.34, No.12, p.1237-1241


Phenylenediamine isomers

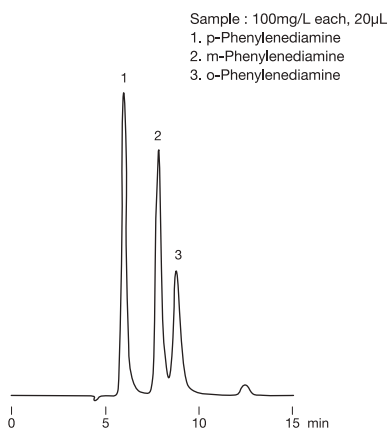

Sample : 100mg/L each, 20μL
 1. p-Phenylenediamine
 2. m-Phenylenediamine
 3. o-Phenylenediamine

Column : Shodex RSpak JJ-50 4D
Eluent : 25mM Ammonium acetate buffer
 (pH9.2)/CH₃CN=70/30
Flow rate : 0.4mL/min
Detector : UV (254nm)
Column temp. : 30°C

High sensitive analysis of bromate by LC/MS/MS

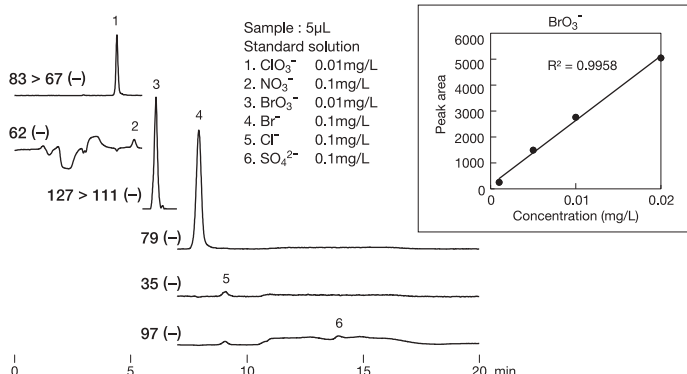

Sample : 5μL
 Standard solution
 1. ClO₃⁻ 0.01mg/L
 2. NO₃⁻ 0.1mg/L
 3. BrO₃⁻ 0.01mg/L
 4. Br⁻ 0.1mg/L
 5. Cl⁻ 0.1mg/L
 6. SO₄²⁻ 0.1mg/L

Column : Shodex RSpak JJ-50 2D
Eluent : (A); 200mM HCOONH₄ aq./ (B); CH₃CN
 Linear gradient (High pressure);
 (B%) 85% (0min) → 85% (8min) → 50% (9min) → 50% (14min)
 → 85% (15min) → 85% (20min)
Flow rate : 0.3mL/min
Detector : ESI-MS/MS (MRM) for ClO₃⁻, BrO₃⁻
 ESI-MS (SIM) for NO₃⁻, Br⁻, Cl⁻, SO₄²⁻
Column temp. : 50°C

Polymer-based Hydrophilic Interaction Chromatography (HILIC) Columns (HILICpak)

Features

- VG-50**
- Suitable for saccharides analysis using HILIC mode
 - Recovers reducing saccharides with high ratio
 - Polymer-based packing material provides excellent chemical stability and minimum deterioration over extended time period
 - Easily regenerated by washing in an alkaline solution
 - Appropriate for evaporative light scattering detector, corona charged aerosol detector, and LC/MS
- VT-50**
- Suitable for anionic substances analysis using HILIC mode
 - Use of some eluents add ion exchange mode
 - Polymer-based packing material provides excellent chemical stability and minimum deterioration over extended time period
 - Suitable for LC/MS analysis
- New VC-50**
- Modified carboxyl group is suitable for cationic substance analysis including amines
 - The dominant separation mode is RP or IEX rather than HILIC mode
- New VN-50**
- The modified diol groups on the packing material create the HILIC mode
 - Suitable for oligosaccharide separation which is not possible by SEC column or conventional HILIC columns

Standard columns

VG-50

(Housing Material: SUS)

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7630200	HILICpak VG-50 4D	≥ 5,500	Amino	5	100	4.6 × 150	H ₂ O/CH ₃ CN=20/80
F7630100	HILICpak VG-50 4E	≥ 7,500	Amino	5	100	4.6 × 250	H ₂ O/CH ₃ CN=20/80
F6711100	HILICpak VG-50G 4A	(guard column)	Amino	5	100	4.6 × 10	H ₂ O/CH ₃ CN=20/80

Base Material: Polyvinyl alcohol

(Housing Material: PEEK)

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7630300	HILICpak VG-50 2D	≥ 3,500	Amino	5	100	2.0 × 150	H ₂ O/CH ₃ CN=15/85
F6711200	HILICpak VG-50G 2A	(guard column)	Amino	5	100	2.0 × 10	H ₂ O/CH ₃ CN=15/85

Base Material: Polyvinyl alcohol

VT-50

(Housing Material: PEEK)

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7630400	HILICpak VT-50 2D	≥ 4,500	Quaternary ammonium	5	100	2.0 × 150	25mM HCOONH ₄ aq. /CH ₃ CN=15/85
F6711300	HILICpak VT-50G 2A	(guard column)	Quaternary ammonium	5	100	2.0 × 10	25mM HCOONH ₄ aq. /CH ₃ CN=15/85

Base Material: Polyvinyl alcohol

VC-50

(Housing Material: PEEK)

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7630700	New HILICpak VC-50 2D	≥ 3,500	Carboxyl	5	100	2.0 × 150	H ₂ O
F6711600	New HILICpak VC-50G 2A	(guard column)	Carboxyl	5	100	2.0 × 10	H ₂ O

Base Material: Polyvinyl alcohol


VN-50

(Housing Material: PEEK)


Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7630600	New HILICpak VN-50 2D	≥ 3,500	Diol	5	100	2.0 × 150	H ₂ O/CH ₃ CN=25/75
F6711500	New HILICpak VN-50G 2A	(guard column)	Diol	5	100	2.0 × 10	H ₂ O/CH ₃ CN=25/75
F7630500	New HILICpak VN-50 4D	≥ 10,000	Diol	5	100	4.6 × 150	H ₂ O/CH ₃ CN=25/75
F6711400	New HILICpak VN-50G 4A	(guard column)	Diol	5	100	4.6 × 10	H ₂ O/CH ₃ CN=25/75

Base Material: Polyvinyl alcohol

Recovery of reducing sugar

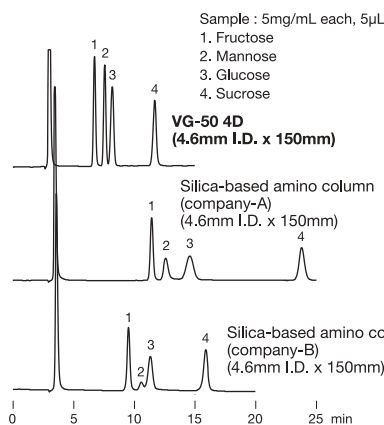


When an amino column is used for analyzing saccharides, the recovery ratio of reducing saccharides such as mannose, arabinose or xylose is low because the amino group forms Schiff base with reducing saccharides. HILICpak VG-50 is an amino column with improved reducing saccharides' recovery ratios. Improved recovery ratio results in enhancing the sensitivity of the analysis.



Column : Shodex HILICpak VG-50 4D
Silica based amino columns from other manufacturers


Eluent : H₂O/CH₃CN=20/80
Flow rate : 0.6mL/min (VG-50 4D)
1.0mL/min (Silica based amino column)
Detector : RI
Column temp. : 40°C

Rare sugar

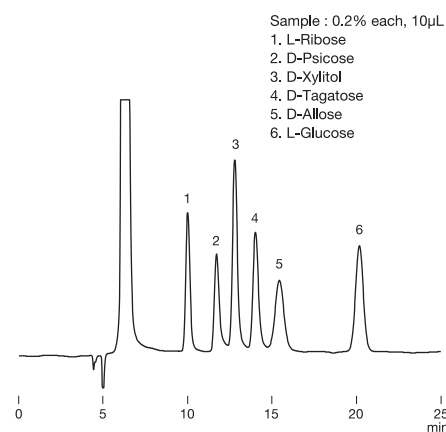


Column : Shodex HILICpak VG-50 4E
Eluent : H₂O/CH₃CN/CH₃OH=5/85/10
Flow rate : 0.6mL/min
Detector : RI
Column temp. : 50°C

Lactose, epilactose, and lactulose

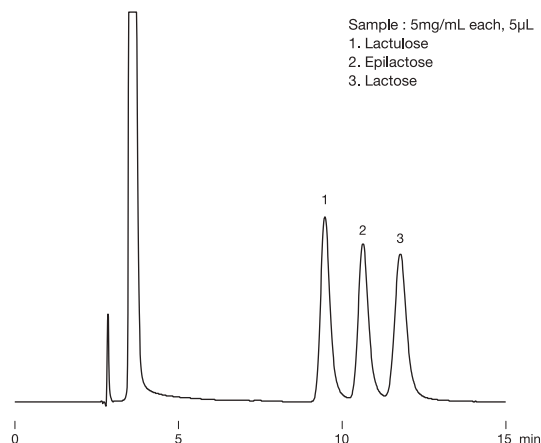


Column : Shodex HILICpak VG-50 4E
Eluent : H₂O/CH₃CN/CH₃OH=5/75/20
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Melamine and related substances

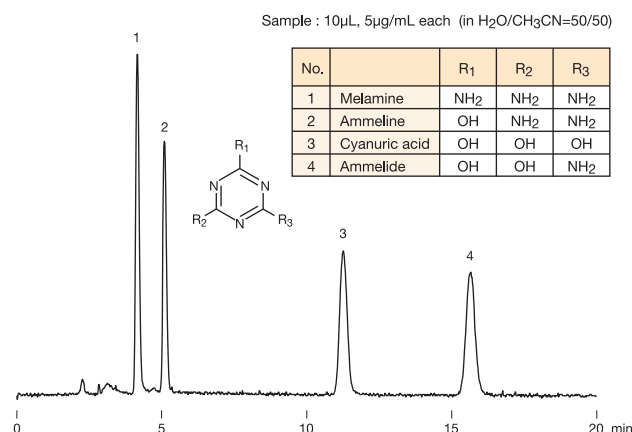

Column : Shodex HILICpak VG-50 4D
Eluent : 30mM HCOONH₄ aq./CH₃CN=35/65
Flow rate : 0.6mL/min
Detector : Corona charged aerosol
Column temp. : 40°C

Simultaneous analysis of saccharides, organic acids and amino acids with LC/MS

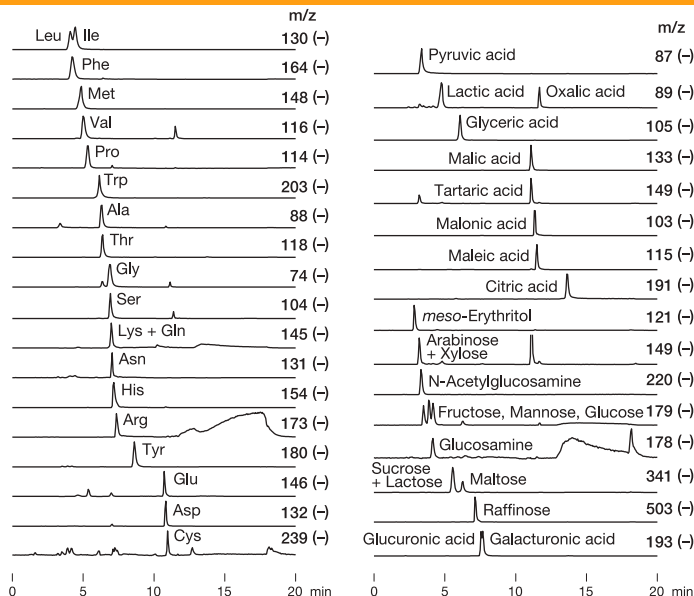


Sample : 1μg/mL each (in H₂O/CH₃CN=1/4), 5μL

VG-50 2D allows simultaneous analysis of saccharides, organic acids and amino acids with LC/MS detection under alkaline conditions. High anionic substances elute under alkaline conditions. Furthermore, alkaline conditions promote the deprotonation of hydroxyl groups at the time of ionization. Therefore, alkaline conditions are suitable for high sensitive detection of substances with hydroxyl groups such as saccharides under the negative mode.


Column : Shodex HILICpak VG-50 2D
Eluent : (A); 0.5% NH₃ aq./ (B); CH₃CN
Linear gradient (High pressure);
(B%) 80% (0 to 2min), 80% to 10% (2 to 12min),
10% (12 to 15min), 80% (15 to 20min)
Flow rate : 0.2mL/min
Detector : ESI-MS (SIM)
Column temp. : 40°C

LC/MS/MS analysis of organic sulfonic acids

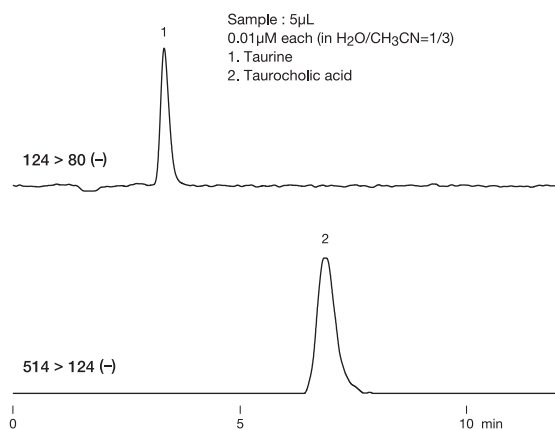


Column : Shodex HILICpak VT-50 2D
Eluent : 50mM HCOONH₄ aq./CH₃CN=20/80
Flow rate : 0.3mL/min
Detector : ESI-MS/MS (MRM)
Column temp. : 30°C

LC/MS analysis of pantothenic acid and vitamin C

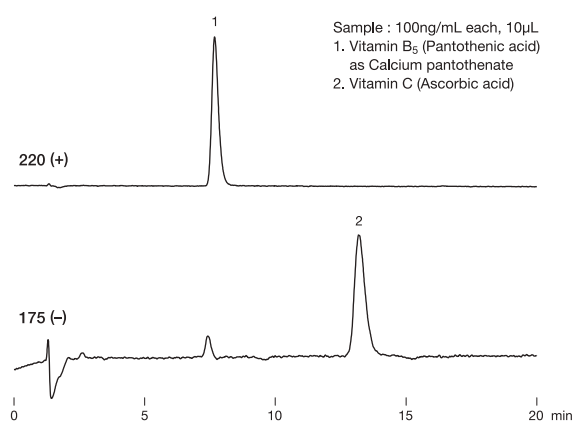


Column : Shodex HILICpak VT-50 2D
Eluent : 50mM HCOONH₄ aq./CH₃CN=30/70
Flow rate : 0.2mL/min
Detector : ESI-MS (SIM)
Column temp. : 30°C

LC/MS analysis of glyphosate and glufosinate

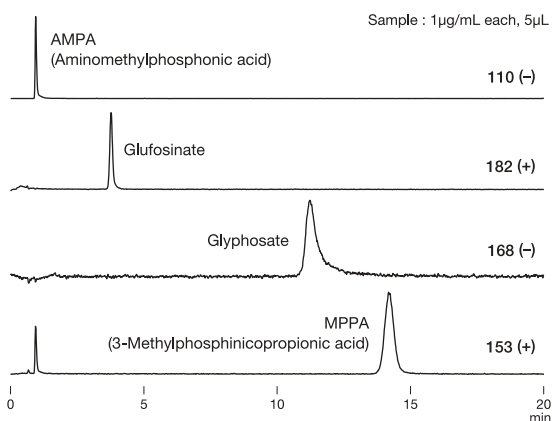


Column : Shodex HILICpak VT-50 2D
Eluent : H₂O/1% HCOOH aq./CH₃CN=70/20/10
Flow rate : 0.3mL/min
Detector : ESI-MS (SIM)
Column temp. : 40°C

LC/MS analysis of phosphorylated saccharides

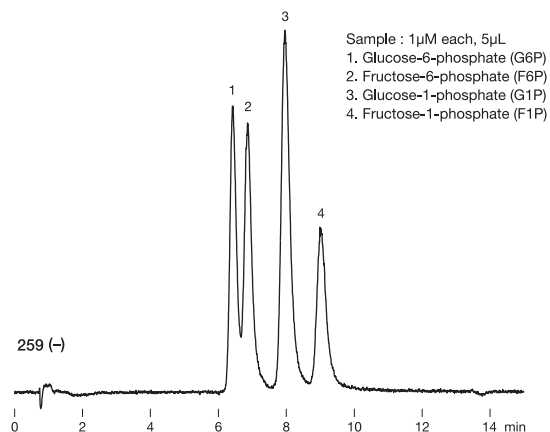


Column : Shodex HILICpak VT-50 2D
Eluent : 25mM HCOONH₄ aq./CH₃CN=80/20
Flow rate : 0.3mL/min
Detector : ESI-MS (SIM)
Column temp. : 60°C

LC/MS analysis of aminoglycoside antibiotics

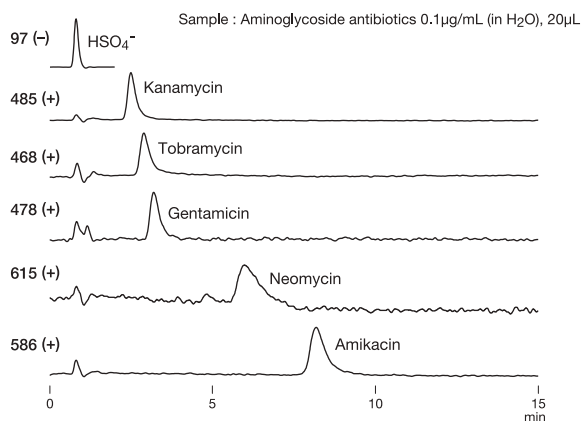


Column : Shodex HILICpak VC-50 2D
Eluent : (A); 1.5% NH₃ aq./ (B); CH₃CN
Linear gradient (High pressure);
(B%) 30% to 10% (0 to 5min), 10% (5 to 15min)
Flow rate : 0.3mL/min
Detector : ESI-MS (SIM)
Column temp. : 40°C

LC/MS/MS analysis of histamine and histidine

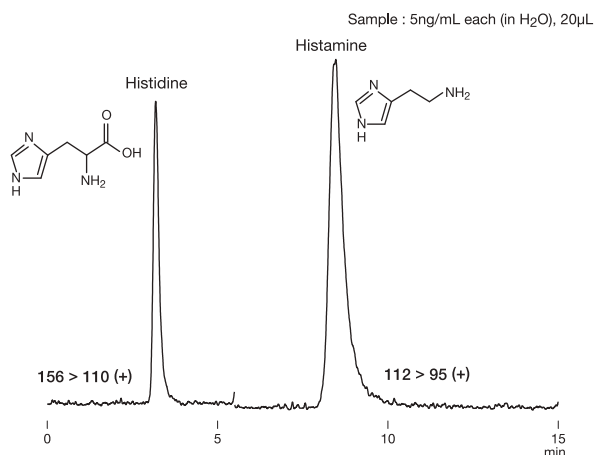


Column : Shodex HILICpak VC-50 2D
Eluent : 250mM HCOOH aq./CH₃CN=70/30
Flow rate : 0.3mL/min
Detector : ESI-MS/MS (MRM)
Column temp. : 40°C

LC/MS/MS analysis of monoamine neurotransmitters

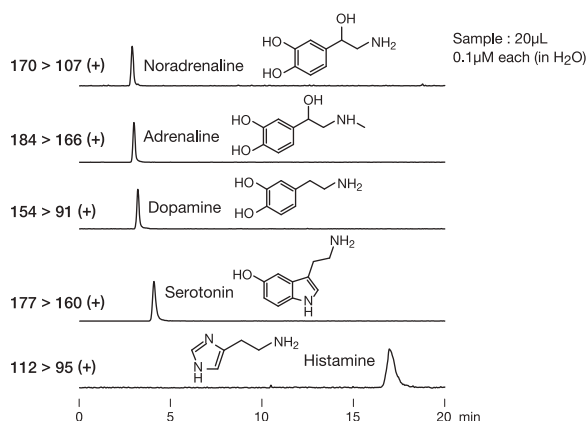


Column : Shodex HILICpak VC-50 2D
Eluent : (A); 200mM HCOOH aq./ (B); CH₃CN
 Linear gradient (High pressure) ;
 (B%) 60% (0 to 5min), 60% to 10% (5 to 6min), 10% (6 to 20min)
Flow rate : 0.3mL/min
Detector : ESI-MS/MS (MRM)
Column temp. : 40°C

LC/MS/MS analysis of oral anti-diabetes drugs

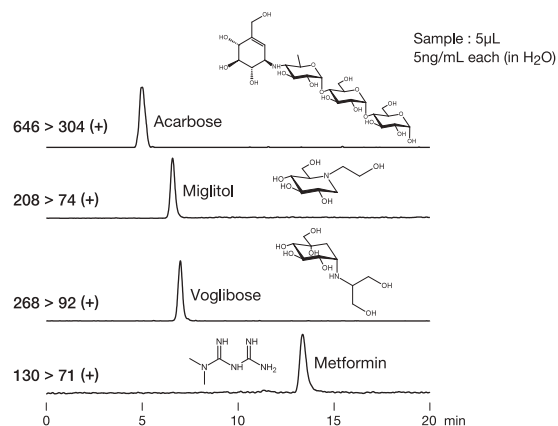

Column : Shodex HILICpak VC-50 2D
Eluent : (A); 200mM HCOOH aq./ (B); CH₃CN
 Linear gradient (High pressure) ;
 (B%) 60% (0 to 5min), 60% to 20% (5 to 6min), 20% (6 to 20min)
Flow rate : 0.3mL/min
Detector : ESI-MS/MS (MRM)
Column temp. : 40°C


LC/MS/MS analysis of ribavirin

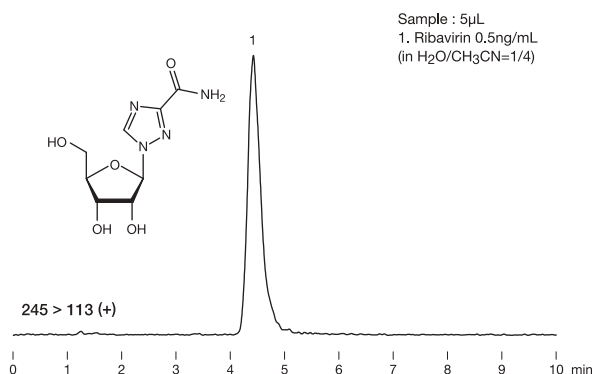

Column : Shodex HILICpak VC-50 2D
Eluent : 50mM HCOOH aq./CH₃CN=10/90
Flow rate : 0.25mL/min
Detector : ESI-MS/MS (MRM)
Column temp. : 40°C


LC/MS analysis of oligo DNA

Sample : 1 μ L
 Synthesized oligo DNA 20mer (ATACCGATTAAGCGAAGTTT; crude)
 2.2mg/mL (in H₂O)

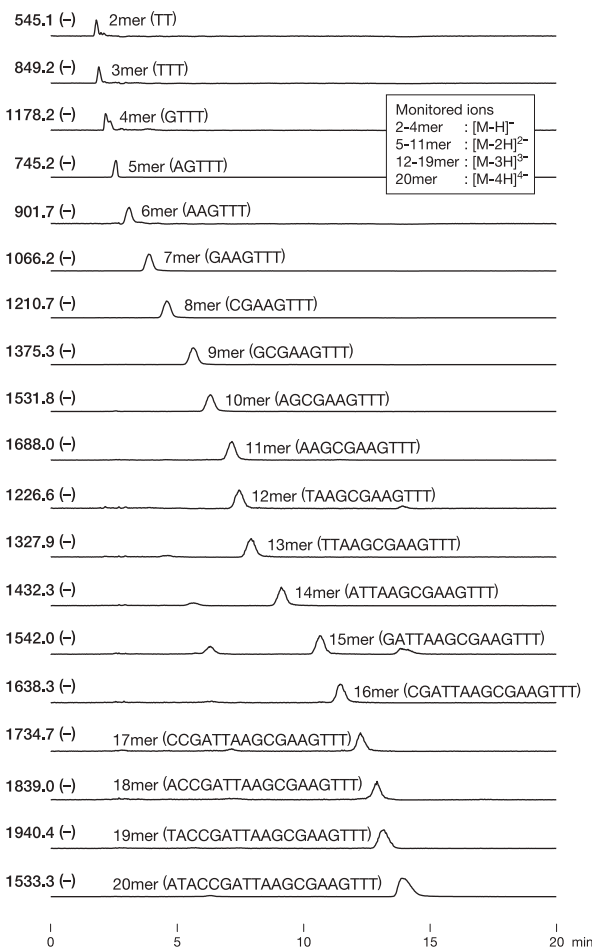

Column : Shodex HILICpak VN-50 2D
Eluent : (A); 50mM HCOONH₄ aq./ (B); CH₃CN
 Linear gradient ;
 (B%) 60% (0 to 10min), 60% to 55% (10 to 15min),
 60% (15 to 20min)
Flow rate : 0.2mL/min
Detector : ESI-MS (SIM)
Column temp. : 40°C

Hydrolyzed dextran

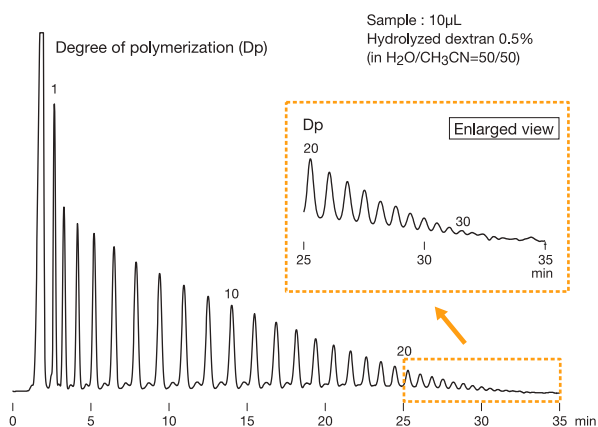

Column : Shodex HILICpak VN-50 4D
Eluent : (A); H₂O/ (B); CH₃CN
 Linear gradient ; (B) 70% to 50% (0 to 40min)
Flow rate : 1.0mL/min
Detector : Corona charged aerosol
Column temp. : 40°C

● Polymer-based Hydrophilic Interaction Chromatography (HILIC) Columns (Asahipak)

Features

- NH2P**
- Suitable for saccharides analysis using HILIC mode
 - Polymer-based packing material provides excellent chemical stability and minimum deterioration over extended time period
 - Easily regenerated by washing in an alkaline solution
 - Appropriate for evaporative light scattering detector, corona charged aerosol detector, and LC/MS
 - Fulfills USP L82 requirements

NH2P-40 • Provides higher theoretical plate number than NH2P-50 series

■ Standard columns

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7630005	Asahipak NH2P-50 4B	≥ 1,500	Amino	5	100	4.6 × 50	CH ₃ CN
F7630002	Asahipak NH2P-50 4D	≥ 5,500	Amino	5	100	4.6 × 150	CH ₃ CN
F7630001	Asahipak NH2P-50 4E	≥ 7,500	Amino	5	100	4.6 × 250	CH ₃ CN
F6710016	Asahipak NH2P-50G 4A	(guard column)	Amino	5	–	4.6 × 10	CH ₃ CN
F7630006	Asahipak NH2P-50 2D	≥ 3,500	Amino	5	100	2.0 × 150	CH ₃ CN
F6713000	Asahipak NH2P-50G 2A	(guard column)	Amino	5	–	2.0 × 10	CH ₃ CN
F7630007	Asahipak NH2P-40 3E	≥ 8,500	Amino	4	100	3.0 × 250	CH ₃ CN
F6710030	Asahipak NH2P-50G 3A	(guard column)	Amino	5	–	3.0 × 10	CH ₃ CN
F7630008	Asahipak NH2P-40 2B	≥ 2,000	Amino	4	100	2.0 × 50	CH ₃ CN
F7630009	Asahipak NH2P-40 2D	≥ 5,500	Amino	4	100	2.0 × 150	CH ₃ CN
F7630010	Asahipak NH2P-40 2E	≥ 7,000	Amino	4	100	2.0 × 250	CH ₃ CN
F6710100	Asahipak NH2P-LF	(line filter)	Amino	–	–	8.0 × 75	CH ₃ CN

Base Material: Polyvinyl alcohol

■ 3mm I.D columns [Customized columns]


Product Code	Product Name	Functional Group	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F7630011	Asahipak NH2P-40 3B	Amino	4	100	3.0 × 50
F7630012	Asahipak NH2P-40 3D	Amino	4	100	3.0 × 150

Base Material: Polyvinyl alcohol

■ Preparative columns *Preparative columns are made to order.


Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6830001	Asahipak NH2P-50 10E	≥ 10,000	5	10.0 × 250	NH2P-50
F6710016	Asahipak NH2P-50G 4A	(guard column)	5	4.6 × 10	(guard column)
F6830031	Asahipak NH2P-90 20F	≥ 10,000	9	20.0 × 300	NH2P-50
F6710017	Asahipak NH2P-130G 7B	(guard column)	13	7.5 × 50	(guard column)

Fructooligosaccharide syrup

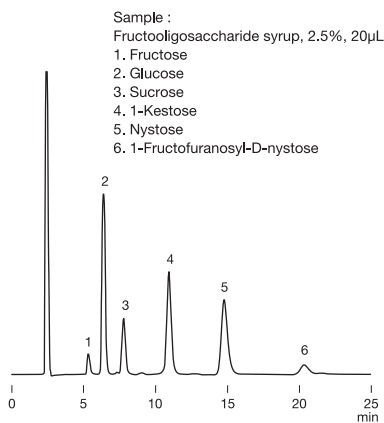


Column : Shodex Asahipak NH2P-50 4E
Eluent : H₂O/CH₃CN=30/70
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 25°C

Cyclodextrins

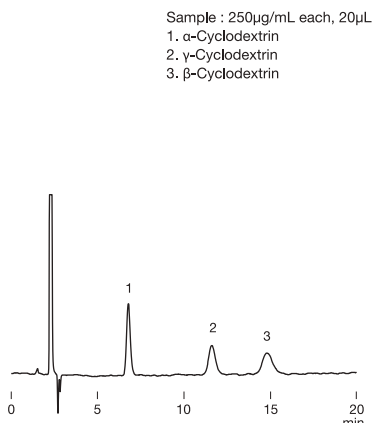


Column : Shodex Asahipak NH2P-50 4E
Eluent : H₂O/CH₃CN=40/60
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Stevioside and rebaudioside A

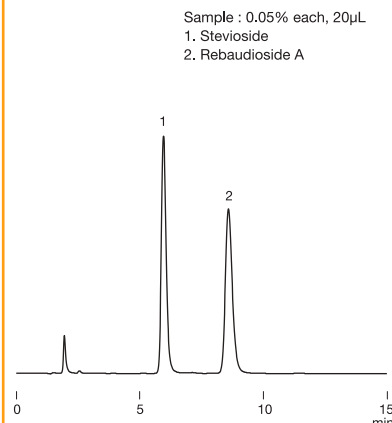


Column : Shodex Asahipak NH2P-50 4E
Eluent : H₂O/CH₃CN=25/75
Flow rate : 1.0mL/min
Detector : UV (210nm)
Column temp. : 30°C

Imidazole dipeptides

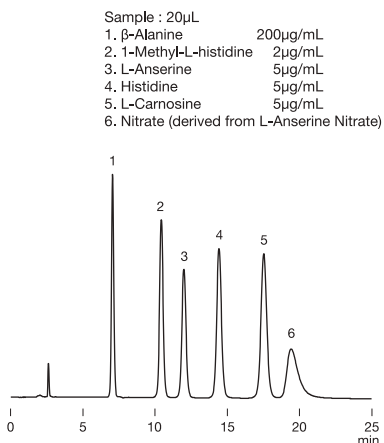


Column : Shodex Asahipak NH2P-50 4E
Eluent : 50mM NaH₂PO₄ aq./CH₃CN=40/60
Flow rate : 1.0mL/min
Detector : UV (210nm)
Column temp. : 40°C

Simultaneous analysis of water-soluble vitamins

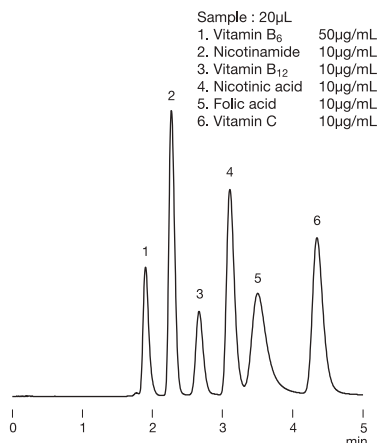


Column : Shodex Asahipak NH2P-50 4E
Eluent : 40mM H₃PO₄ aq./CH₃CN=45/55
Flow rate : 1.0mL/min
Detector : UV (254nm)
Column temp. : 40°C

Ascorbic acid and erythorbic acid

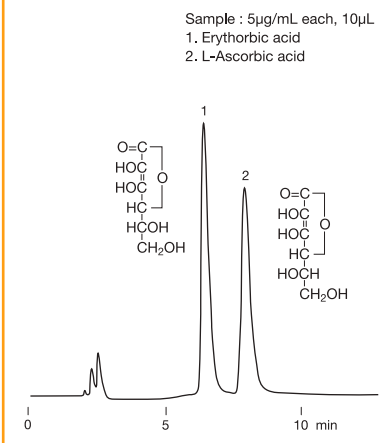


Column : Shodex Asahipak NH2P-50 4E
Eluent : 20mM NaH₂PO₄ + 30mM H₃PO₄ aq./CH₃CN=20/80
Flow rate : 1.0mL/min
Detector : UV (254nm)
Column temp. : 30°C

Comparison of saccharide analysis using corona charged aerosol detector

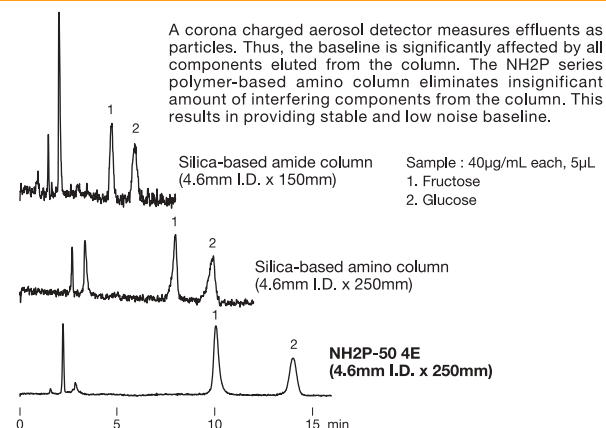

Column : Shodex Asahipak NH2P-50 4E
Silica based amino column from other manufacturer
Silica based amide column from other manufacturer
Eluent : H₂O/CH₃CN=20/80
Flow rate : 1.0mL/min
Detector : Corona charged aerosol
Column temp. : 30°C (NH2P-50 4E, Silica based amino column)
80°C (Silica based amide column)

LC/TOF-MS analysis of 2-amino benzoic acid derivatized sugar chains

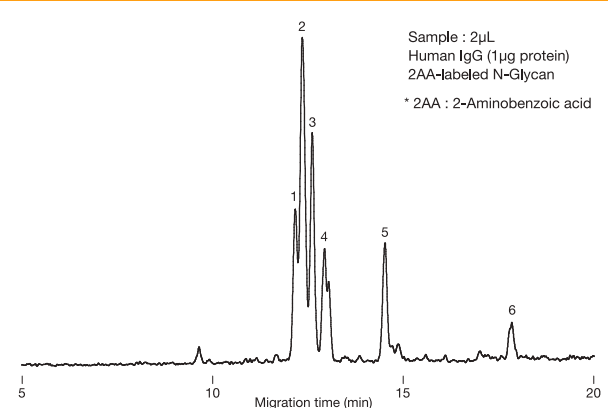

Column : Shodex Asahipak NH2P-40 2D
Eluent : (A); 95% CH₃CN/0.1% Formic acid aq.
(B); 5% CH₃CN/0.1% Formic acid aq.
Linear gradient; (B%) 30% (0-2.5min), 30-95% (2.5-20min)
Flow rate : 0.2mL/min
Detector : ESI-TOF MS (Polarity : Negative, Full MS range : 2000)
Column temp. : 45°C

Data provided by Michihiro Kinoshita Ph.D.,
Faculty of Pharmacy, Kinki University

● Silica-based Reversed Phase Chromatography Columns (ODS Columns)

Please refer to "Comparison of Shodex Reversed Phase Chromatography (RPC) Column Features" on page 6 and 7 for features.

■ Standard columns

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Carbon Load (%)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6651010	C18-4D*	≥ 13,000	Octadecyl	5	17	120	4.6 × 150	H ₂ O/CH ₃ OH=25/75
F6651011	C18-4E *	≥ 21,000	Octadecyl	5	17	120	4.6 × 250	H ₂ O/CH ₃ OH=25/75
F6650040	Silica C18M 4D	≥ 10,000	Octadecyl	5	16	100	4.6 × 150	H ₂ O/CH ₃ OH=30/70
F6650041	Silica C18M 4E	≥ 16,000	Octadecyl	5	16	100	4.6 × 250	H ₂ O/CH ₃ OH=30/70
F6650042	Silica C18M 2D	≥ 9,000	Octadecyl	5	16	100	2.0 × 150	H ₂ O/CH ₃ CN=40/60
F6650045	Silica C18P 4D	≥ 10,000	Octadecyl	5	17	100	4.6 × 150	H ₂ O/CH ₃ OH=30/70
F6650046	Silica C18P 4E	≥ 16,000	Octadecyl	5	17	100	4.6 × 250	H ₂ O/CH ₃ OH=30/70
F6650047	Silica C18P 2D	≥ 9,000	Octadecyl	5	17	100	2.0 × 150	H ₂ O/CH ₃ CN=40/60

*Only available in bundles of 10 ea.

Base Material: Silica

■ Preparative columns *Preparative columns are made to order.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F7560040	Silica C18M 10E	≥ 16,000	5	10.0 × 250	C18M
F7560041	Silica C18M 20E	≥ 16,000	5	20.0 × 250	C18M

● Silica-based Reversed Phase Chromatography Columns (Other Columns)

Please refer to "Comparison of Shodex Reversed Phase Chromatography (RPC) Column Features" on page 6 and 7 for features.

■ Standard columns

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Carbon Load (%)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6650052	Silica 5C8 4D	≥ 9,000	Octyl	5	10	100	4.6 × 150	H ₂ O/CH ₃ OH=34/66
F6650053	Silica 5C8 4E	≥ 15,000	Octyl	5	10	100	4.6 × 250	H ₂ O/CH ₃ OH=34/66
F6650058	Silica 5CN 4D	≥ 7,000	Cyanopropyl	5	-	100	4.6 × 150	H ₂ O/CH ₃ OH=60/40
F6650059	Silica 5CN 4E	≥ 12,000	Cyanopropyl	5	-	100	4.6 × 250	H ₂ O/CH ₃ OH=60/40
F6650062	Silica 5NPE 4D	≥ 8,000	Nitrophenylethyl	5	-	100	4.6 × 150	H ₂ O/CH ₃ OH=45/55
F6650063	Silica 5PYE 4D	≥ 7,000	Pyrenylethyl	5	-	100	4.6 × 150	H ₂ O/CH ₃ OH=30/70

Base Material: Silica

■ Preparative columns *Preparative columns are made to order.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F7560062	Silica 5C8 10E	≥ 15,000	5	10.0 × 250	5C8
F7560063	Silica 5C8 20E	≥ 15,000	5	20.0 × 250	5C8

● Silica-based Normal Phase Chromatography and HILIC Columns

Features

- 5SIL**
- Packed with high purity silica (99.99% or higher)
 - Suitable used with nonpolar organic solvents for normal phase analysis
 - Fulfills USP L3 requirements
-
- 5NH**
- Suitable for saccharides analysis using HILIC mode
 - Fulfills USP L8 requirements

■ Standard columns


Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Carbon Load (%)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6650050	Silica 5SIL 4D	≥ 9,000	–	5	–	100	4.6 × 150	C ₆ H ₁₄ /C ₂ H ₅ OH=95/5
F6650051	Silica 5SIL 4E	≥ 15,000	–	5	–	100	4.6 × 250	C ₆ H ₁₄ /C ₂ H ₅ OH=95/5
F6650060	Silica 5NH 4D	≥ 5,000	Aminopropyl	5	–	100	4.6 × 150	H ₂ O/CH ₃ CN=5/95
F6650061	Silica 5NH 4E	≥ 8,000	Aminopropyl	5	–	100	4.6 × 250	H ₂ O/CH ₃ CN=5/95

Base Material: Silica

■ Preparative columns *Preparative columns are made to order.


Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F7560050	Silica 5SIL 10E	≥ 15,000	5	10.0 × 250	5SIL
F7560051	Silica 5SIL 20E	≥ 15,000	5	20.0 × 250	5SIL
F7560060	Silica 5NH 10E	≥ 8,000	5	10.0 × 250	5NH
F7560061	Silica 5NH 20E	≥ 8,000	5	20.0 × 250	5NH

Fat-soluble vitamins

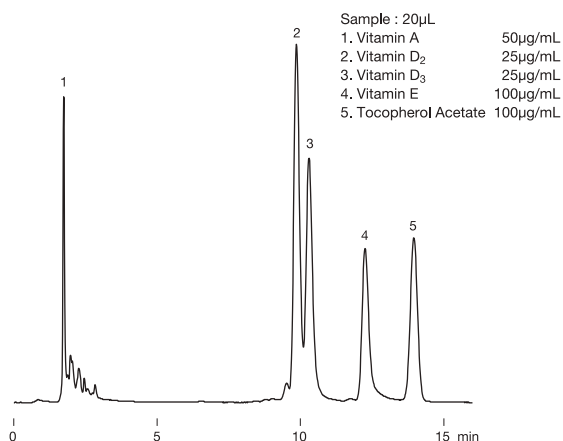


Column : Shodex C18-4D
Eluent : CH₃CN
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : 40°C

Anticonvulsant

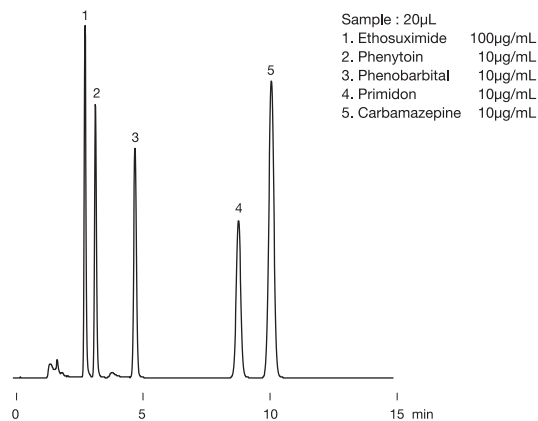


Column : Shodex C18-4D
Eluent : 100mM Phosphate buffer(pH2.1)
 /CH₃OH/CH₃CN=4/2/1
Flow rate : 1.0mL/min
Detector : UV (210nm)
Column temp. : 40°C

Aflatoxins

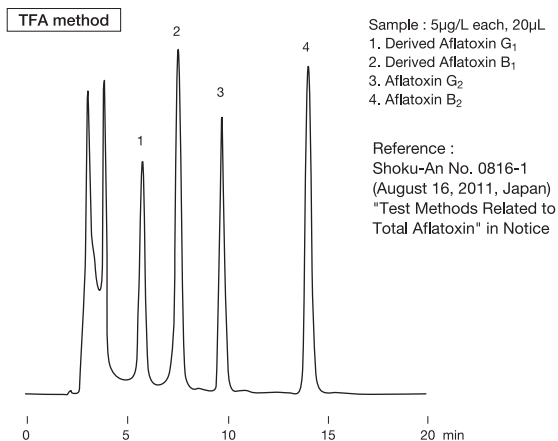


Column : Shodex Silica C18M 4E
Eluent : H₂O/CH₃CN/CH₃OH=60/10/30
Flow rate : 1.0mL/min
Detector : Fluorescence (Ex. : 365nm, Em. : 450nm)
Column temp. : 40°C

Trichothecene mycotoxins

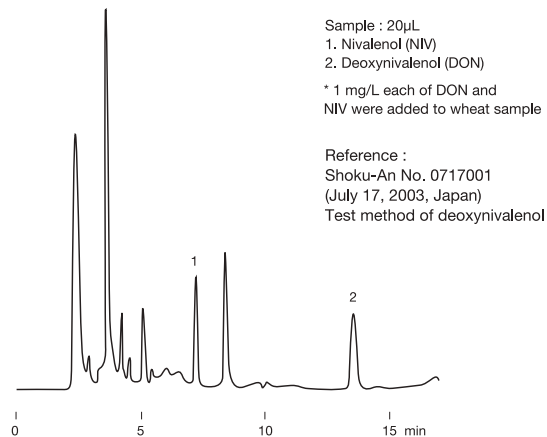


Column : Shodex Silica C18M 4E
Eluent : H₂O/CH₃CN/CH₃OH=90/5/5
Flow rate : 1.0mL/min
Detector : UV (220nm)
Column temp. : 40°C

Gingerol and shogaol

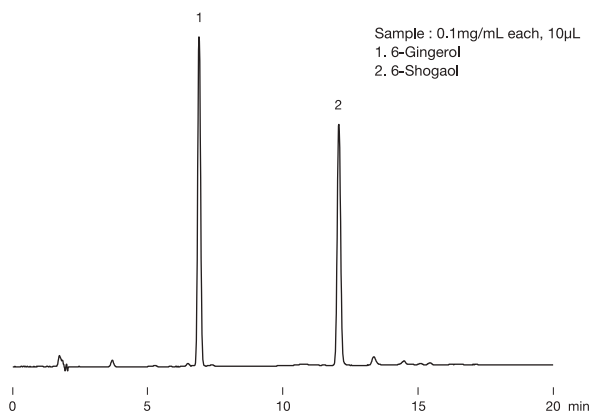

Column : Shodex Silica C18M 4D
Eluent : (A) : H₂O (B) : CH₃CN
 Linear gradient : (B%) 40% to 70% (15min)
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : 40°C


Chlorogenic acid

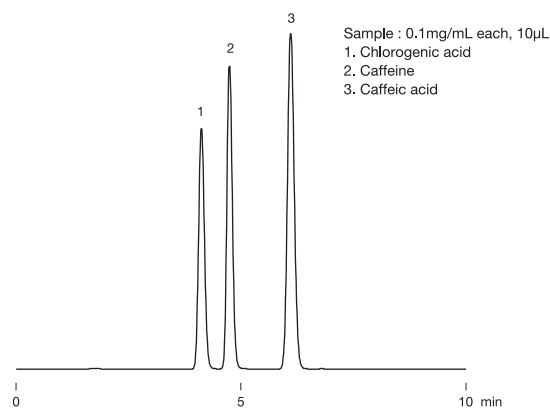

Column : Shodex Silica C18M 4D
Eluent : 20mM H₃PO₄ aq. /CH₃OH=70/30
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : 30°C

Catechins


Sample : 10µg/mL each, 10µL
 1. Epigallocatechin
 2. Catechin
 3. Epigallocatechingallate
 4. Epicatechin
 5. Epicatechingallate
 6. Catechingallate

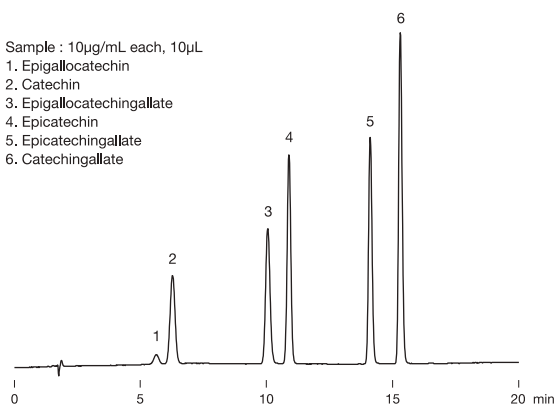

Column : Shodex Silica C18P 4D
Eluent : (A) ; 20mM H₃PO₄ aq./ (B) ; CH₃CN
 Linear gradient:
 (B%) 20% (0 to 5min), 20 to 40% (5 to 15min),
 40% (15 to 20min)
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : 30°C

Estrogens


Sample : 0.1mg/mL each, 10µL
 1. Estriol
 2. 17β-Estradiol
 3. Estrone

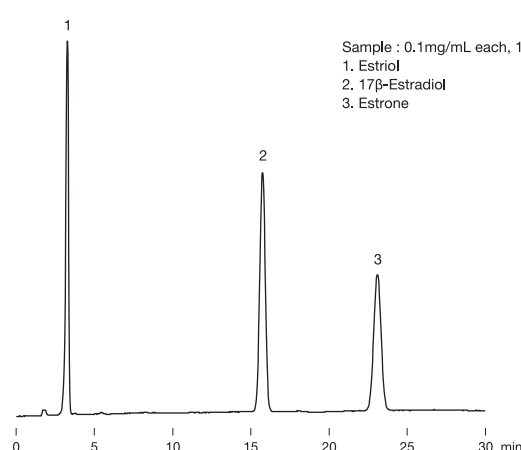

Column : Shodex Silica C18P 4D
Eluent : H₂O/CH₃CN=65/35
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : 30°C

Analysis of glucosamine following USP method


Sample : 10µL
 3.8 mg/mL Glucosamine hydrochloride
 (in H₂O/CH₃CN=1/1)
 1. Cl⁻
 2. Glucosamine

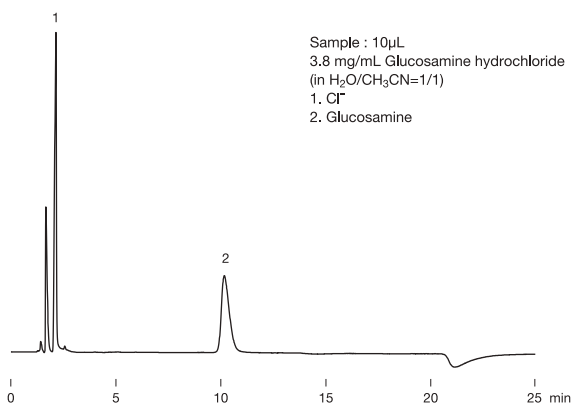

Column : Shodex Silica 5NH 4D
Eluent : *Buffer(pH7.5)/CH₃CN=30/70
 *Buffer; in a 1-L volumetric flask, dissolve 3.5g K₂HPO₄ in water.
 Add 0.25mL Ammonium hydroxide (25%), dilute with water to
 volume, and mix. Adjusted with H₃PO₄ to a pH7.5
Flow rate : 1.1mL/min
Detector : UV (195nm)
Column temp. : 35°C

Benzylpyridine isomers


Sample :
 1. 2-Benzylpyridine
 2. 3-Benzylpyridine
 3. 4-Benzylpyridine

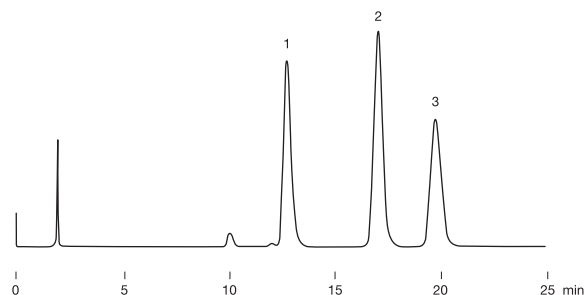

Column : Shodex Silica 5PYE 4D
Eluent : 20mM KH₂PO₄ aq./CH₃OH=40/60
Flow rate : 1.0mL/min
Detector : UV (254nm)
Column temp. : 30°C

Dinitronaphthalene isomers


Sample :
 1. Naphthalene
 2. 1,5-Dimethylnaphthalene
 3. 1,5-Dinitronaphthalene
 4. 1,8-Dinitronaphthalene

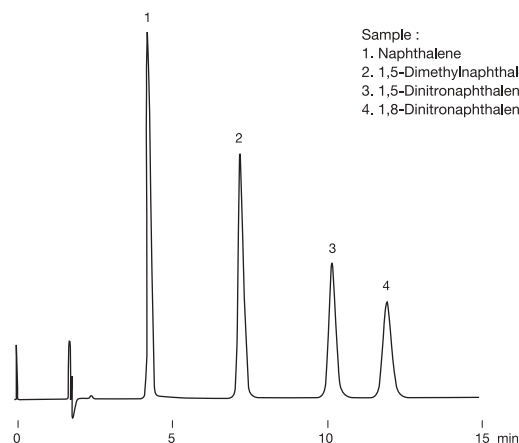

Column : Shodex Silica 5NPE 4D
Eluent : H₂O/CH₃OH=30/70
Flow rate : 1.0mL/min
Detector : UV (254nm)
Column temp. : 30°C

Simultaneous analysis of vitamin E homologs

Sample : 20µL
 1. α-Tocopherol 5µg/mL
 2. α-Tocotrienol 10µg/mL
 3. β-Tocopherol 5µg/mL
 4. γ-Tocopherol 5µg/mL
 5. γ-Tocotrienol 10µg/mL
 6. δ-Tocopherol 5µg/mL
 7. δ-Tocotrienol 10µg/mL

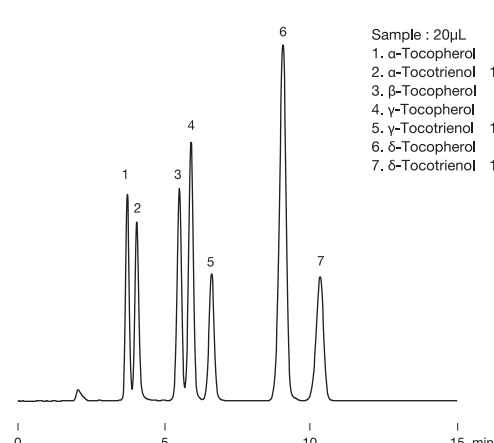

Column : Shodex Silica 5SIL 4D
Eluent : n-Hexane/Isopropanol/CH₃COOH=1000/6/5
Flow rate : 1.0mL/min
Detector : Fluorescence (Ex. : 298nm, Em. : 325nm)
Column temp. : 30°C

Ligand Exchange Chromatography Columns

Lists summarizing elution volumes of various saccharides using Shodex columns is available. Please refer to our website (<http://www.shodex.com/en/>) or technical notebook (No.2 and 3).

Features

- | | |
|---|--|
| SC1011
SC1821
SP0810
KS-801 to 802 | <ul style="list-style-type: none"> • Separates saccharides by combination of ligand exchange and size exclusion modes • Three types of counter ions are available: Ca²⁺, Pb²⁺, and Na⁺ • Only water is required for the analysis of neutral sugars • SC1011 and SC1821 fulfill USP L19 and L22 requirements • SP0810 fulfills USP L22 and L34 requirements • KS-801 and KS-802 fulfill USP L22 and L58 requirements |
| KS-803 to 806 | <ul style="list-style-type: none"> • Suitable for separation of polysaccharides by size exclusion mode • Can be used in combination with other columns e.g., KS-802 and KS-801 • Only water is required for the analysis of neutral sugars • Fulfills USP L22 and L58 requirements |
| DC-613
SZ5532
SC1211 | <ul style="list-style-type: none"> • Separates elements by combination of ligand exchange and HILIC modes • DC-613 can analyze sugars without removing sodium salts in the sample • SZ5532 is recommended for the separation of disaccharides or trisaccharides • SC1211 is suitable for separating sugar alcohols • DC-613 fulfills USP L22 and L58 requirements • SZ5532 fulfills USP L22 requirements • SC1211 fulfills USP L19 and L22 requirements |
| SC1011-7F | <ul style="list-style-type: none"> • Fulfills mannitol analysis requirements of JP, USP, and EP methods • Ca²⁺ modified ligand exchange chromatography column • Only water is required for the analysis of neutral sugars • Fulfills USP L19 and L22 requirements |

Standard columns

[Ligand exchange and size exclusion]

Product Code	Product Name	Plate Number (TP/column)	Functional Group (Counter Ion)	Exclusion Limit (Pullulan)	Particle Size (μm)	Column Size (mm) I.D. x Length	Shipping Solvent
F6378102	SUGAR SC1011	≥ 13,000	Sulfo (Ca ²⁺)	1,000	6	8.0 × 300	H ₂ O
F6378103	SUGAR SC1821	≥ 13,000	Sulfo (Ca ²⁺)	10,000	6	8.0 × 300	H ₂ O
F6700090	SUGAR SC-G 6B (SUGAR SC-LG)	(guard column)	Sulfo (Ca ²⁺)	—	10	6.0 × 50	H ₂ O
F6378105	SUGAR SP0810	≥ 11,000	Sulfo (Pb ²⁺)	1,000	7	8.0 × 300	H ₂ O
F6700081	SUGAR SP-G 6B (SUGAR SP-G)	(guard column)	Sulfo (Pb ²⁺)	—	10	6.0 × 50	H ₂ O
F6378010	SUGAR KS-801	≥ 17,000	Sulfo (Na ⁺)	1,000	6	8.0 × 300	H ₂ O
F6378020	SUGAR KS-802	≥ 17,000	Sulfo (Na ⁺)	10,000	6	8.0 × 300	H ₂ O
F6378025	SUGAR KS-803	≥ 17,000	Sulfo (Na ⁺)	50,000	6	8.0 × 300	H ₂ O
F6378035	SUGAR KS-804	≥ 17,000	Sulfo (Na ⁺)	400,000	7	8.0 × 300	H ₂ O
F6378050	SUGAR KS-805	≥ 9,000	Sulfo (Na ⁺)	5,000,000	17	8.0 × 300	H ₂ O
F6378060	SUGAR KS-806	≥ 9,000	Sulfo (Na ⁺)	*(50,000,000)	17	8.0 × 300	H ₂ O
F6700020	SUGAR KS-G 6B (SUGAR KS-G)	(guard column)	Sulfo (Na ⁺)	—	10	6.0 × 50	H ₂ O

*() Estimated value Base Material: Styrene divinylbenzene copolymer

[Ligand exchange and HILIC]

Product Code	Product Name	Plate Number (TP/column)	Functional Group (Counter Ion)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7001003	RSpak DC-613	≥ 5,500	Sulfo (Na ⁺)	6	100	6.0 × 150	H ₂ O/CH ₃ CN=30/70
F6700170	RSpak DC-G 4A (RSpak DC-G)	(guard column)	Sulfo (Na ⁺)	10	—	4.6 × 10	H ₂ O/CH ₃ CN=30/70
F7001300	SUGAR SZ5532	≥ 5,500	Sulfo (Zn ²⁺)	6	—	6.0 × 150	H ₂ O/CH ₃ CN=30/70
F6700110	SUGAR SZ-G	(guard column)	Sulfo (Zn ²⁺)	6	—	4.6 × 10	H ₂ O/CH ₃ CN=30/70
F7001400	SUGAR SC1211	≥ 5,500	Sulfo (Ca ²⁺)	6	50	6.0 × 250	H ₂ O/CH ₃ CN=75/25
F6700120	SUGAR SC1211G 4A (SUGAR SC-G)	(guard column)	Sulfo (Ca ²⁺)	10	—	4.6 × 10	H ₂ O/CH ₃ CN=75/25

Base Material: Styrene divinylbenzene copolymer

For mannitol analysis following JP, USP, and EP methods

Product Code	Product Name	Functional Group (Counter Ion)	Particle Size (μm)	Column Size (mm) I.D. x Length	Shipping Solvent
F6379300	EP SC1011-7F	Sulfo (Ca ²⁺)	8	7.8 × 300	H ₂ O
F6700090	SUGAR SC-G 6B (SUGAR SC-LG) (guard column)	Sulfo (Ca ²⁺)	10	6.0 × 50	H ₂ O
F6379230	USPpak MN-431	Sulfo (Ca ²⁺)	8	4.0 × 250	H ₂ O

*See page 79 for USP40-NF35 Column List.

Base Material: Styrene divinylbenzene copolymer

Preparative columns *Preparative columns are made to order.

[Ligand exchange and size exclusion]

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6502007	SUGAR KS-2001	≥ 7,000	13	20.0 × 300	KS-801
F6502008	SUGAR KS-2002	≥ 7,000	13	20.0 × 300	KS-802
F6502009	SUGAR KS-2003	≥ 8,000	13	20.0 × 300	KS-803
F6502010	SUGAR KS-2004	≥ 6,000	18	20.0 × 300	KS-804
F6502011	SUGAR KS-2005	≥ 6,000	18	20.0 × 300	KS-805
F6502012	SUGAR KS-2006	≥ 6,000	18	20.0 × 300	KS-806
F6700002	SUGAR KS-G 8B (SUGAR KS-LG)	(guard column)	13	8.0 × 50	(guard column)

[Ligand exchange and HILIC]

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6514013	RSpak DC-2013	≥ 6,000	10	20.0 × 300	DC-613
F6700402	RSpak DC-G 8B (RSpak DC-LG)	(guard column)	10	8.0 × 50	(guard column)

Elution volumes of saccharides analyzed by Shodex columns

[Partial list only; refer to our website for complete list]

Substances	Elution Volume (mL)					
	SP0810	SC1011	KS-801	SZ5532	NH2P-50 4E	SC1211
Arabinose	10.42	8.91	8.21	5.11	6.18	5.56
D-Arabitol	15.86	11.33	7.63	7.27	6.29	8.16
Dulcitol	20.18	12.76	7.40	9.46	7.45	11.28
meso-Erythritol	12.70	10.09	7.86	5.73	5.43	6.27
D(-)-Fructose	11.05	8.85	7.71	5.37	6.75	5.90
D(+)-Fucose	10.48	8.84	8.09	4.50	5.43	4.96
D(+)-Galactose	9.74	7.98	7.58	6.46	8.10	4.98
Gentiobiose	7.22	6.08	5.75	10.50	16.36	*
Glucose	8.63	7.30	7.17	5.87	8.61	4.76
myo-Inositol	12.77	8.86	7.99	12.63	9.96	7.87
Isomaltose	7.68	6.26	5.95	10.57	15.18	*
Isomaltotriose	7.09	5.75	5.34	21.17	27.55	*
1-Kestose	6.79	5.75	5.26	13.09	20.11	*
Kojibiose	7.56	6.21	5.88	9.65	14.82	*
Lactitol	13.27	8.09	6.13	16.35	11.82	6.67
Lactose	8.05	6.51	5.99	10.12	13.27	4.07
Lactulose	9.13	6.99	6.19	9.16	10.72	4.65
Maltitol	12.23	8.26	6.03	13.04	11.82	6.77
Maltose	7.85	6.34	5.94	8.67	14.24	*
Maltotriose	7.48	5.89	5.38	13.79	24.96	*
Mannitol	15.80	11.10	7.23	8.75	7.39	9.03

(-)→Not detected (-)→Overlap with solvent peak

Substances	Elution Volume (mL)					
	SP0810	SC1011	KS-801	SZ5532	NH2P-50 4E	SC1211
D-Mannose	10.72	8.17	7.64	5.83	7.84	5.01
Melibiose	8.16	6.45	5.98	11.69	14.70	4.23
Nystose	6.38	5.45	4.93	20.05	31.90	*
Palatinin	2peaks	2peaks	5.90	2peaks	12.73	2peaks
Palatinose	7.84	6.45	5.89	8.08	12.12	3.99
Panose	7.14	5.78	5.32	16.87	25.60	*
D(+)-Raffinose	7.14	5.78	5.29	16.36	20.25	*
Rhamnose	9.77	8.23	7.37	3.93	5.52	4.43
D(-)-Ribose	19.35	13.66	9.04	4.82	5.45	8.64
D(-)-Sorbitol	21.61	13.31	7.42	9.79	7.09	11.88
Sorbose	9.67	8.03	7.38	5.12	7.35	4.92
Stachyose	6.82	5.57	4.97	—	36.22	*
Sucrose	7.54	6.29	5.87	7.91	11.87	*
α-D-Talose	21.33	12.59	8.76	5.69	6.47	8.51
Trehalose	7.62	6.27	5.78	10.85	13.25	*
Trehalulose	8.92	6.95	6.10	9.54	11.68	4.78
Xylitol	19.87	13.14	7.94	7.77	6.10	10.16
Xylobiose	8.16	6.68	6.40	5.65	9.05	*
D(+)-Xylose	9.21	7.90	7.71	4.55	6.58	4.48
D-Xylulose	10.64	9.02	8.04	4.06	5.41	5.07

(-)→Not detected (-)→Overlap with solvent peak

Column : SUGAR SP0810, SC1011, KS-801
Eluent : H₂O
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 80°C

Column : SUGAR SC1211
Eluent : H₂O/CH₃CN=65/35
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 70°C


Column : SUGAR SZ5532
Eluent : H₂O/CH₃CN=25/75
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 60°C

Column : Asahipak NH2P-50 4E
Eluent : H₂O/CH₃CN=25/75
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 30°C

Saccharides anomer separation


Saccharides may present their anomers at lower temperatures. By setting the SUGAR series columns at higher temperatures will prevent the anomer separation and this results in providing better chromatograms of each saccharide.

Sample :
0.5% each, 10 μ L

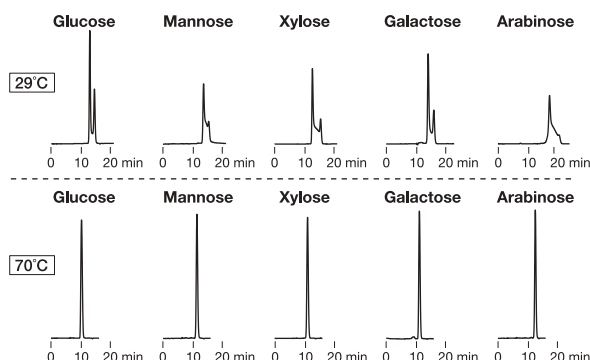


Column : Shodex SUGAR SC1011
Eluent : H₂O
Flow rate : 0.7mL/min
Detector : RI
Column temp. : 29°C, 70°C

Calibration curves for KS-800 series using pullulan

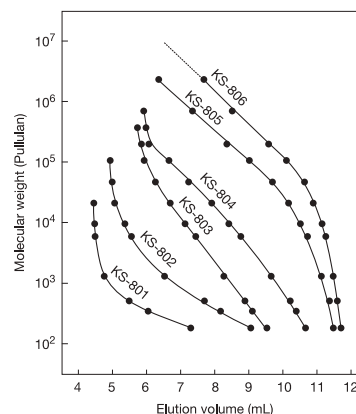

Column : Shodex SUGAR KS-800 series
Eluent : H₂O
Detector : RI
Column temp. : 80°C


Hydrolyzed starch

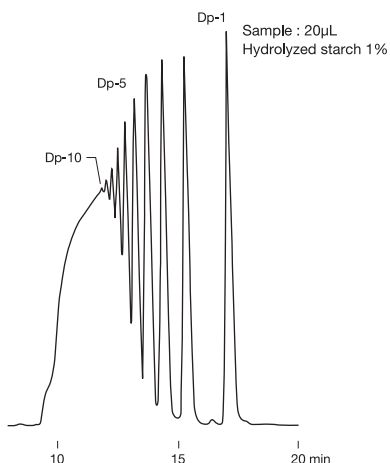

Sample : 20 μ L
Hydrolyzed starch 1%
Column : Shodex SUGAR KS-802 x 2
Eluent : H₂O
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 80°C

Biomass sugars


Sample : 5 μ L
1. Cellobiose 1.0%
2. Glucose 1.5%
3. Xylose 0.5%
4. Galactose 0.5%
5. Arabinose 0.5%
6. Mannose 1.0%

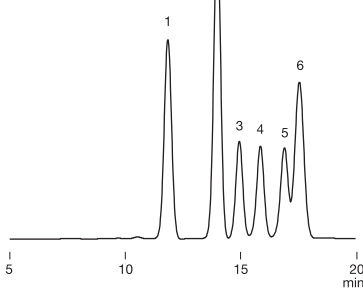

Column : Shodex SUGAR SP0810
Eluent : H₂O
Flow rate : 0.6mL/min
Detector : RI
Column temp. : 85°C

Ketohexoses


Sample : 0.025% each, 10 μ L
1. Sorbose
2. Fructose
3. Tagatose
4. Psicose

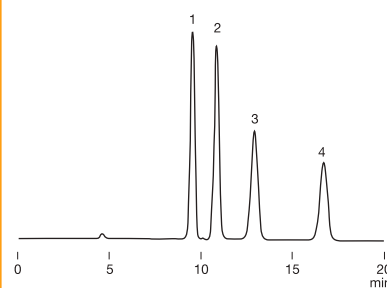

Column : Shodex SUGAR SP0810
Eluent : H₂O
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 80°C

Pinitol


Sample : 0.1% each, 20 μ L
1. Sucrose
2. Glucose
3. Pinitol
4. Fructose
5. *chiro*-Inositol
6. *myo*-Inositol

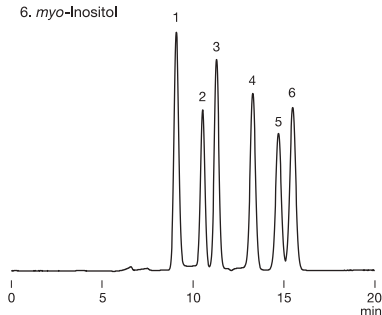

Column : Shodex SUGAR SP0810
Eluent : H₂O
Flow rate : 0.8mL/min
Detector : RI
Column temp. : 85°C

Oligosaccharides in soybean


Sample : 0.1% each, 20 μ L
1. Verbascose
2. Stachyose
3. Raffinose
4. Sucrose
5. Pinitol

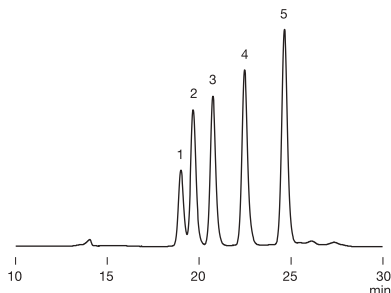

Column : Shodex SUGAR KS-802 + KS-801
Eluent : H₂O
Flow rate : 0.6mL/min
Detector : RI
Column temp. : 85°C

Saccharides related to raffinose biosynthesis


Sample : 0.1% each, 20 μ L
1. Raffinose
2. Sucrose
3. Galactinol
4. Galactose
5. *myo*-Inositol

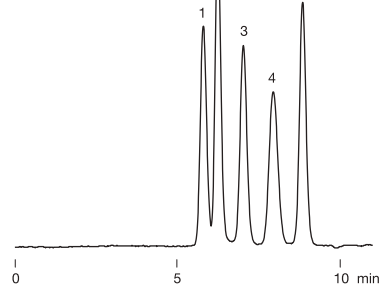

Column : Shodex SUGAR SC1011
Eluent : H₂O
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 80°C

Acesulfame K and sucralose


Sample : 20 μ L
 1. Acesulfame K 0.1%
 2. Sucrose 0.5%
 3. Glucose 0.5%
 4. Unknown from Acesulfame K
 5. Fructose 0.5%
 6. Sucralose 0.1%

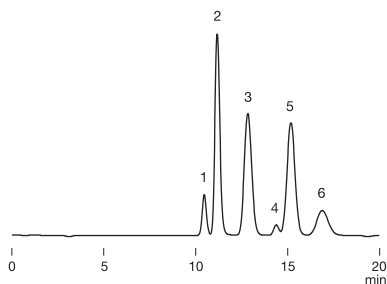

Column : Shodex SUGAR SC1011
 Eluent : 10mM CaSO₄ aq.
 Flow rate : 0.6mL/min
 Detector : RI
 Column temp. : 80°C

Sucrose and turanose


Sample : 0.5% each, 10 μ L
 1. Fructose
 2. Glucose
 3. Sucrose
 4. Turanose
 5. Lactose

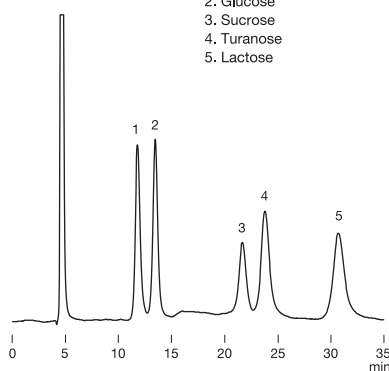

Column : Shodex SUGAR SZ5532
 Eluent : H₂O/CH₃CN=20/80
 Flow rate : 0.6mL/min
 Detector : RI
 Column temp. : 60°C

Maltose and isomaltose


Sample : 0.5% each, 20 μ L
 1. Glucose
 2. Maltose
 3. Isomaltose
 4. Maltotriose
 5. Isomaltotriose

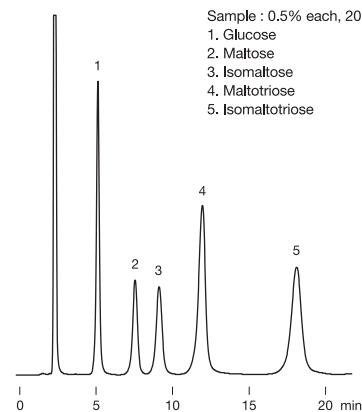

Column : Shodex SUGAR SZ5532
 Eluent : H₂O/CH₃CN=25/75
 Flow rate : 1.0mL/min
 Detector : RI
 Column temp. : 60°C

Saccharides and sugar alcohols


Sample : 0.5% each, 20 μ L
 1. Rhamnose
 2. Xylose
 3. Arabinose
 4. Fructose
 5. Glucose
 6. Galactose
 7. Arabinol
 8. Xylitol
 9. Mannitol
 10. Sorbitol

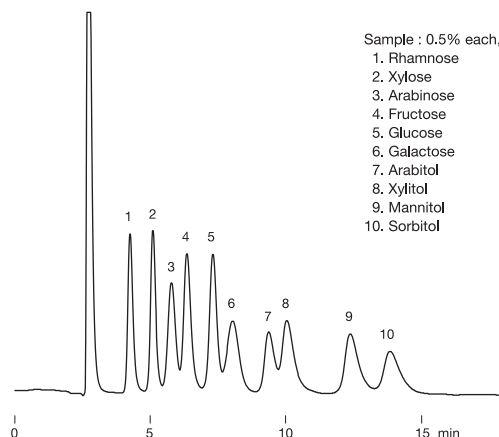

Column : Shodex SUGAR SZ5532
 Eluent : H₂O/CH₃CN=20/80
 Flow rate : 1.0mL/min
 Detector : RI
 Column temp. : 65°C

Saccharides and taurine


Sample : 0.1% each, 20 μ L
 1. Sucrose
 2. Glucose
 3. Fructose
 4. Taurine
 5. *myo*-Inositol

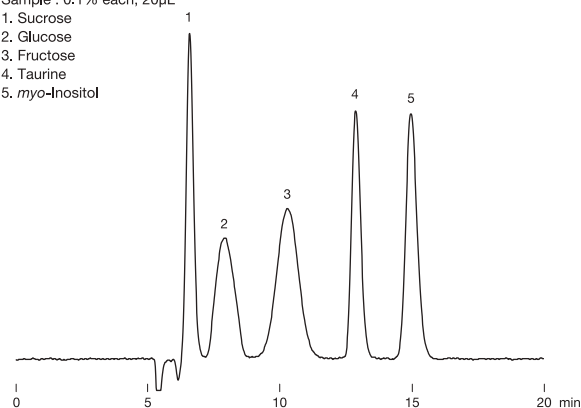

Column : Shodex SUGAR SC1211
 Eluent : H₂O/CH₃CN=60/40
 Flow rate : 0.6mL/min
 Detector : RI
 Column temp. : 70°C

Moisturizing components

Sample : 0.1% each, 20 μ L
 1. 1,3-Propanediol
 2. Propylene glycol
 3. Ethylene glycol
 4. Glycerin
 5. *meso*-Erythritol

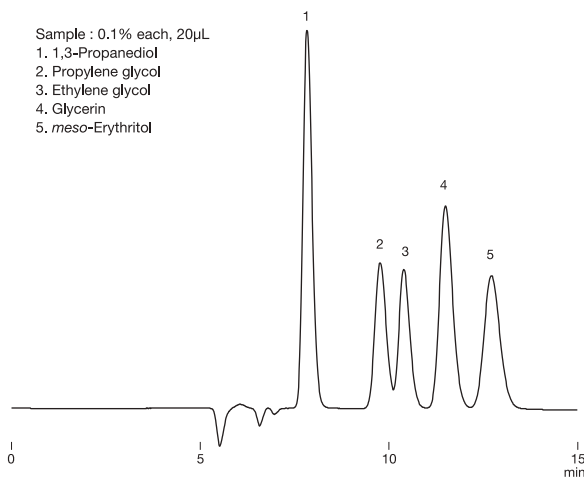


Column : Shodex SUGAR SC1211
 Eluent : H₂O/CH₃CN=60/40
 Flow rate : 0.6mL/min
 Detector : RI
 Column temp. : 40°C

Mannitol and sorbitol

Partial modifications on the analytical conditions of mannitol stated in the United States Pharmacopeia (USP, USP37-NF32) became effective on December 1st, 2014. Now for the separation of mannitol and sorbitol, USP, European Pharmacopeia (EP), and Japanese Pharmacopeia (JP) request to use a column having resolution more than 2.0. SC1011-7F fulfills the conditions required from USP, EP, and JP.

Sample : 25mg/mL each, 20 μ L
 1. Mannitol
 2. Sorbitol

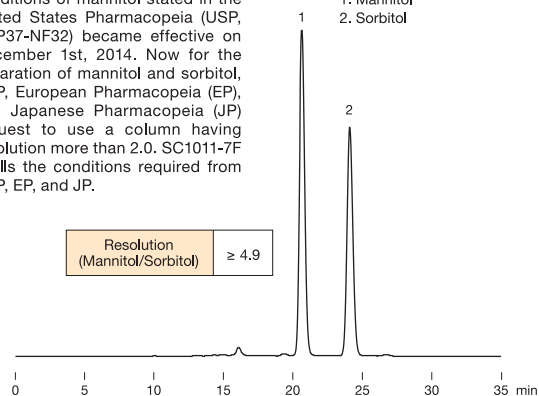

Column : Shodex EP SC1011-7F
 Eluent : H₂O
 Flow rate : 0.5mL/min
 Detector : RI
 Column temp. : 85°C

● Ion Exclusion Chromatography Columns

Features

- SH1011** • Columns for simultaneous analysis of saccharides and organic acids
 - SH1821** • Separates neutral sugars in size exclusion mode and organic acids in ion exclusion mode
 - Suitable for the analysis of uronic and aldonic acids
 - Fulfills USP L17 and L22 requirements
-
- KC-811** • Columns suitable for the analysis of organic acids
 - Separates compounds by ion exclusion mode and reversed phase mode
 - Highly selective when used with post column method
 - KC-811 6E is suitable for the analysis of cyanide ions and cyanogen chloride in accordance with the Japanese Water Supply Act
 - Fulfills USP L17 and L22 requirements

■ Standard columns

[For simultaneous analysis of saccharides and organic acids]

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Exclusion Limit (Pullulan)	Particle Size (μm)	Column Size (mm) I.D. x Length	Shipping Solvent
F6378100	SUGAR SH1011	≥ 17,000	Sulfo	1,000	6	8.0 x 300	H ₂ O
F6378101	SUGAR SH1821	≥ 17,000	Sulfo	10,000	6	8.0 x 300	H ₂ O
F6700080	SUGAR SH-G	(guard column)	Sulfo	–	10	6.0 x 50	H ₂ O

Base Material: Styrene divinylbenzene copolymer

[For organic acids, cyanide ions and cyanogen chloride]

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Column Size (mm) I.D. x Length	Shipping Solvent
F6378030	RSpak KC-811	≥ 17,000	Sulfo	6	8.0 x 300	0.1% H ₃ PO ₄ aq.
F6378033	RSpak KC-811 6E	≥ 13,000	Sulfo	6	6.0 x 250	0.1% H ₃ PO ₄ aq.
F6700030	RSpak KC-G 6B (RSpak KC-G)	(guard column)	Sulfo	10	6.0 x 50	0.1% H ₃ PO ₄ aq.
F6700010	RSpak KC-G 8B (RSpak KC-LG)	(guard column)	Sulfo	13	8.0 x 50	0.1% H ₃ PO ₄ aq.

*Use KC-G 8B for samples with relatively high impurity and KC-G 6B for samples with relatively low impurity.

Base Material: Styrene divinylbenzene copolymer


■ Preparative columns *Preparative columns are made to order.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6505012	RSpak KC-2011	≥ 8,000	13	20.0 x 300	KC-811
F6700010	RSpak KC-G 8B (RSpak KC-LG)	(guard column)	13	8.0 x 50	(guard column)

Maltooligosaccharides, organic acids and ethanol

Sample : 0.05% each, 20 μ L

1. Maltotetraose
2. Maltotriose
3. Maltose
4. Glucose
5. Lactic acid
6. Glycerol
7. Acetic acid
8. Methanol
9. Ethanol

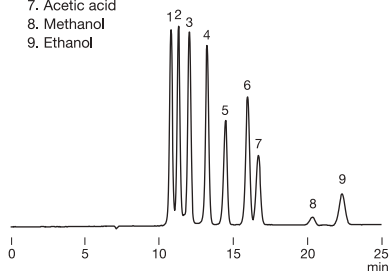


Column : Shodex SUGAR SH1821
Eluent : 0.5mM H₂SO₄ aq.
Flow rate : 0.6mL/min
Detector : RI
Column temp. : 75°C

Cello-oligosaccharides and furfurals

Sample : 0.1% each, 10 μ L

1. Cellopentaose
2. Cellotetraose
3. Cellotriose
4. Cellobiose
5. Glucose
6. Glyceric acid
7. Acetic acid
8. 5-HMF
9. Furfural

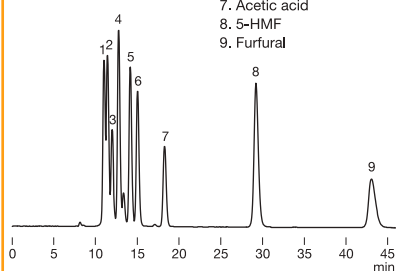


Column : Shodex SUGAR SH1821
Eluent : 2mM H₂SO₄ aq.
Flow rate : 0.6mL/min
Detector : RI
Column temp. : 60°C

Glycerin and glyceric acid

Sample : 0.1% each, 10 μ L

1. Glyceric acid
2. Glycerin

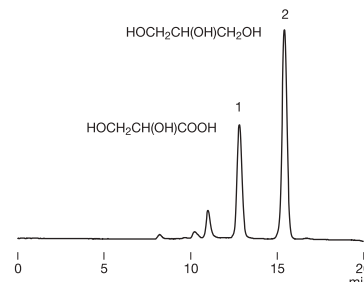


Column : Shodex SUGAR SH1011
Eluent : 2mM H₂SO₄ aq.
Flow rate : 0.6mL/min
Detector : RI
Column temp. : 60°C

Common organic acids

Sample :

1. Citric acid
2. Tartaric acid
3. Pyruvic acid
4. Malic acid
5. Succinic acid
6. Glycolic acid
7. Lactic acid
8. Fumaric acid
9. Acetic acid
10. Levulinic acid
11. Pyroglutamic acid
12. Propionic acid
13. Isobutyric acid
14. n-Butyric acid

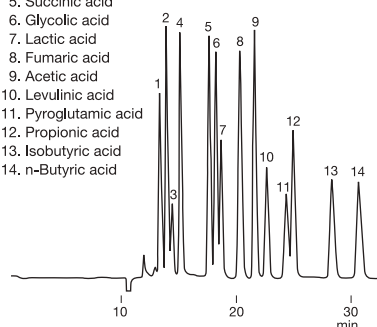


Column : Shodex RSpak KC-811 x 2
Eluent : 6mM HClO₄ aq.
Flow rate : 1.0mL/min
Detector : VIS (430nm)
 post column method
Column temp. : 50°C

Hydrophobic organic acids

Sample :

1. Succinic acid
2. Lactic acid
3. Formic acid
4. Acetic acid
5. Propionic acid
6. Isobutyric acid
7. n-Butyric acid
8. Isovaleric acid
9. n-Valeric acid

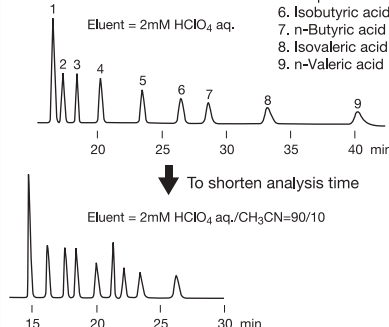


Column : Shodex RSpak KC-LG + KC-811 x 2
Flow rate : 1.0mL/min
Detector : VIS (430nm)
 post column method
Column temp. : 47°C

Glucronolactone and organic acids

Sample : 20 μ L

1. Citric acid 0.01%
2. Malic acid 0.01%
3. Glucronolactone 0.01%
4. Glycerin 0.01%
5. Ethanol 0.05%

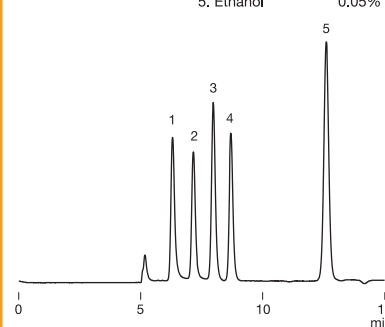


Column : Shodex RSpak KC-811
Eluent : 3mM HClO₄ aq.
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Organic acids in sake

Sample : 100 μ L


1. Phosphoric acid etc.
2. Citric acid
3. Pyruvic acid
4. Malic acid
5. Succinic acid
6. Lactic acid
7. Fumaric acid
8. Acetic acid
9. Pyroglutamic acid

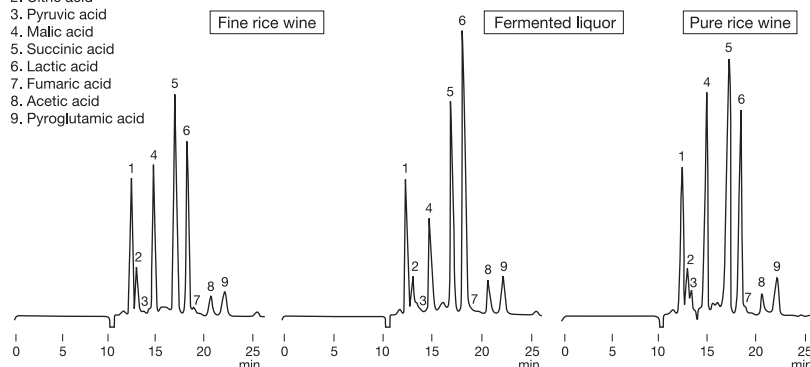

Column : Shodex RSpak KC-LG + KC-811 x 2
Eluent : 4.8mM HClO₄ aq.
Flow rate : 1.0mL/min
Detector : VIS (430nm)
 post column method
Column temp. : 63°C

Analysis of Cyanide ion and cyanogen chloride with post column method

Sample : 10 μ g/L each, 100 μ L

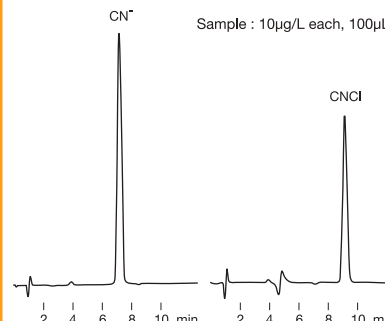

Column : Shodex RSpak KC-811 6E
Eluent : 1.0mM H₂SO₄ aq.
Reagent A : Chloramine T solution
Reagent B : 4-Pyridinecarboxylic acid-Pyrazolone solution
Flow rate : (Eluent) 1.0mL/min
 (Reagent) 0.5mL/min each
Detector : VIS (638nm)
Column temp. : 40°C
Reaction temp. : (Reagent A) 40°C
 (Reagent B) 80°C

● Ion Chromatography Columns (Anion Analysis)

Features

- NI-424 I-524A**
 - Columns for anion analysis with non-suppressor method
 - NI-424 provides simultaneous analysis of fluoride and phosphate ions
- SI-90 4E SI-50 4E**
 - Columns for anion analysis with suppressor method
 - Suitable for the quantitative analysis of fluoride ion
 - SI-50 separates target inorganic anions from organic acids
 - Not interfered by the system peak derived from carbonate
- SI-52 4E**
 - Column for the analysis of oxyhalides with suppressor method
 - Provides simultaneous analysis of oxyhalides and general inorganic ions
- SI-35**
 - Columns for rapid analysis with suppressor method
 - SI-35 4D provides rapid analysis of oxyhalides and general inorganic ions
 - SI-35 2B provides rapid analysis of general inorganic ions

■ Standard columns

[For anion non-suppressor method]

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Column Size (mm) I.D. x Length	Shipping Solvent
F6995243	IC NI-424	≥ 5,000	Quaternary ammonium	5	4.6 × 100	8mM 4-Hydroxybenzoic acid + 2.8mM Bis-Tris + 2mM Phenylboronic acid + 0.005mM CyDTA aq.
F6709616	IC NI-G	(guard column)	Quaternary ammonium	5	4.6 × 10	8mM 4-Hydroxybenzoic acid + 2.8mM Bis-Tris + 2mM Phenylboronic acid + 0.005mM CyDTA aq.
F6995240	IC I-524A	≥ 2,000	Quaternary ammonium	12	4.6 × 100	2.5mM Phthalic acid aq.
F6700400	IC IA-G	(guard column)	Quaternary ammonium	12	4.6 × 10	2.5mM Phthalic acid aq.

[For anion suppressor method]

Base Material: Polyhydroxymethacrylate Housing Material: SUS

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Column Size (mm) I.D. x Length	Shipping Solvent
F6995244	IC SI-90 4E	≥ 5,000	Quaternary ammonium	9	4.0 × 250	1.8mM Na ₂ CO ₃ + 1.7mM NaHCO ₃ aq.
F6709620	IC SI-90G	(guard column)	Quaternary ammonium	9	4.6 × 10	1.8mM Na ₂ CO ₃ + 1.7mM NaHCO ₃ aq.
F6995245	IC SI-50 4E	≥ 10,000	Quaternary ammonium	5	4.0 × 250	3.2mM Na ₂ CO ₃ + 1.0mM NaHCO ₃ aq.
F6709625	IC SI-50G	(guard column)	Quaternary ammonium	5	4.6 × 10	3.2mM Na ₂ CO ₃ + 1.0mM NaHCO ₃ aq.

[For oxyhalides suppressor method]

Base Material: Polyvinyl alcohol Housing Material: PEEK

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Column Size (mm) I.D. x Length	Shipping Solvent
F6995260	IC SI-52 4E	≥ 14,000	Quaternary ammonium	5	4.0 × 250	3.6mM Na ₂ CO ₃ aq.
F6709626	IC SI-92G	(guard column)	Quaternary ammonium	9	4.6 × 10	3.6mM Na ₂ CO ₃ aq.

[For rapid suppressor method]

Base Material: Polyvinyl alcohol Housing Material: PEEK

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Column Size (mm) I.D. x Length	Shipping Solvent
F6995290	IC SI-35 4D	≥ 13,000	Quaternary ammonium	3.5	4.0 × 150	3.6mM Na ₂ CO ₃ aq.
F6709627	IC SI-95G	(guard column)	Quaternary ammonium	9	4.6 × 10	3.6mM Na ₂ CO ₃ aq.
F6995291	IC SI-35 2B	≥ 4,000	Quaternary ammonium	3.5	2.0 × 50	1.0mM Na ₂ CO ₃ + 2.0mM NaHCO ₃ aq.

Base Material: Polyvinyl alcohol Housing Material: PEEK

■ Guard filter for SI-35 2B

Product Code	Product Name	Contents
F6709720	IC SI-2GF	One holder and one filter
F6709730	IC SI-2GF filter	3 filters

Removes insoluble components in the sample

■ Line filters for IC


Product Code	Product Name	Contents
F8500630	IC FL-1	One holder and one filter
F8500640	IC FL-1 filter	5 filters



*Attach directly to analysis column

Removes insoluble components in the eluent by installing it upstream of the injector


Anion analysis using NI-424 and I-524A (non-suppressor methods)

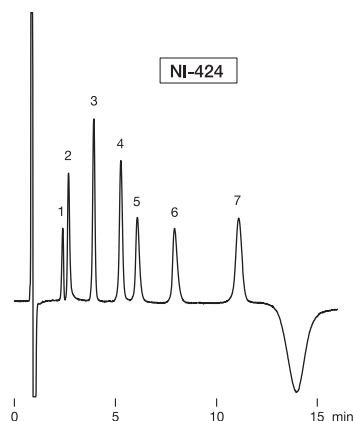

Column : Shodex IC NI-424
Eluent : 8mM 4-Hydroxybenzoic acid + 2.8mM Bis-Tris
 + 2mM Phenylboronic acid + 0.005mM *CyDTA aq.
Flow rate : 1.0mL/min
Detector : Non-suppressed conductivity
Column temp. : 40°C

*CyDTA : trans-1,2-Diaminocyclohexane-N,N,N',N'-tetra acetic acid

Sample : 20μL
 1. H₂PO₄⁻ 10mg/L
 2. F⁻ 1mg/L
 3. Cl⁻ 1mg/L
 4. NO₂⁻ 5mg/L
 5. Br⁻ 5mg/L
 6. NO₃⁻ 5mg/L
 7. SO₄²⁻ 5mg/L

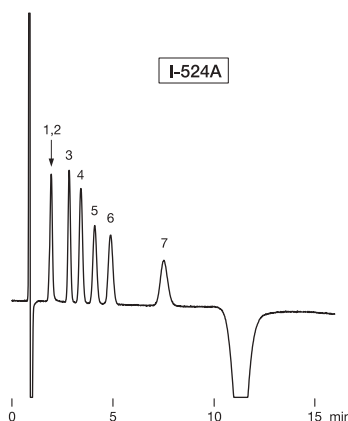

Column : Shodex IC I-524A
Eluent : 2.5mM Phthalic acid
 + 2.3mM Tris(hydroxymethyl)aminomethane aq.
Flow rate : 1.2mL/min
Detector : Non-suppressed conductivity
Column temp. : 40°C


With twice increased theoretical plate number, NI-424 provides a higher performance compared to I-524A.

[Features of NI-424]

- (1) Enables the separation of H₂PO₄⁻ and F⁻ which were difficult to separate with I-524A.
- (2) Provides sharper peaks, and resolution between all peaks are well defined. Especially, the separation of Cl⁻ and NO₂⁻ is improved.

Anion analysis using SI-90 4E (suppressor method)

Sample : 20μL
 1. F⁻ 2mg/L
 2. Cl⁻ 3mg/L
 3. NO₂⁻ 5mg/L
 4. Br⁻ 10mg/L
 5. NO₃⁻ 10mg/L
 6. HCO₃⁻ 300mg/L
 7. PO₄³⁻ 15mg/L
 8. SO₄²⁻ 15mg/L

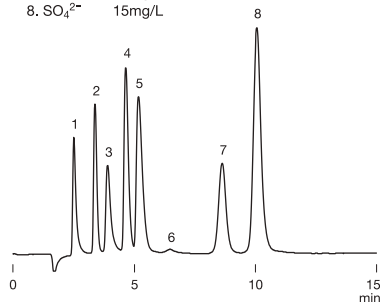


Column : Shodex IC SI-90 4E
Eluent : 1.8mM Na₂CO₃ + 1.7mM NaHCO₃ aq.
Flow rate : 1.5mL/min
Detector : Suppressed conductivity
Column temp. : Room temp. (25°C)

Anion analysis using SI-50 4E (suppressor method)

SI-50 4E is a high performance type of SI-90 4E. Acetic acid, formic acid, and methacrylic acid eluted between F⁻ and Cl⁻. The carbonate system peak appears between NO₂⁻ and Br⁻ peaks.


Sample : 20μL
 1. F⁻ 2mg/L
 2. Acetic acid 10mg/L
 3. Formic acid 2mg/L
 4. Methacrylic acid 10mg/L
 5. Cl⁻ 3mg/L
 6. NO₂⁻ 5mg/L
 7. Br⁻ 10mg/L
 8. NO₃⁻ 10mg/L
 9. PO₄³⁻ 15mg/L
 10. SO₄²⁻ 15mg/L
 11. Oxalic acid 15mg/L

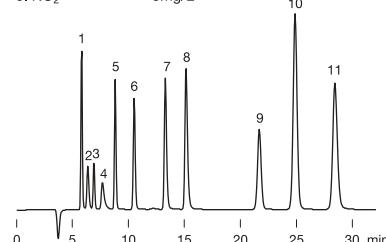

Column : Shodex IC SI-50 4E
Eluent : 3.2mM Na₂CO₃ + 1.0mM NaHCO₃ aq.
Flow rate : 0.7mL/min
Detector : Suppressed conductivity
Column temp. : 25°C

Oxyhalides and anion analysis using SI-52 4E (suppressor method)


SI-52 4E is a high resolution column offering 14,000 or higher theoretical plate number. It supports simultaneous analysis of oxyhalides and inorganic anions. It is recommended to set the column temperature at 45°C.

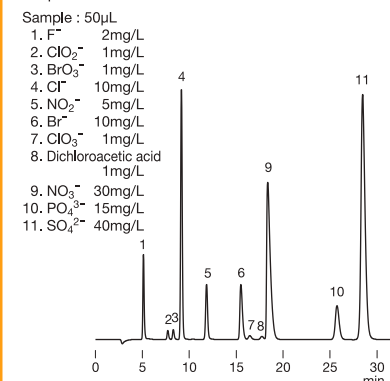

Column : Shodex IC SI-52 4E
Eluent : 3.6mM Na₂CO₃ aq.
Flow rate : 0.8mL/min
Detector : Suppressed conductivity
Column temp. : 45°C

Rapid analysis of oxyhalides and anions using SI-35 4D (suppressor method)


Sample : 20μL
 1. F⁻ 2mg/L
 2. ClO₂⁻ 1mg/L
 3. BrO₃⁻ 1mg/L
 4. Cl⁻ 10mg/L
 5. NO₂⁻ 5mg/L
 6. Br⁻ 10mg/L
 7. ClO₃⁻ 1mg/L
 8. NO₃⁻ 30mg/L
 9. PO₄³⁻ 15mg/L
 10. SO₄²⁻ 40mg/L

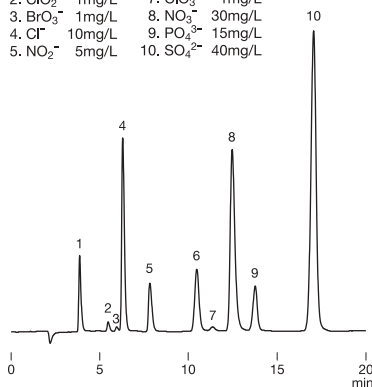

Column : Shodex IC SI-35 4D
Eluent : 2.0mM Na₂CO₃ + 4.5mM NaHCO₃ aq.
Flow rate : 0.6mL/min
Detector : Suppressed conductivity
Column temp. : 45°C

Tricarboxylic acids analysis (suppressor method)


Sample : 20μL
 1. Citric acid 10mg/L
 2. Isocitric acid 50mg/L
 3. trans-Aconitic acid 20mg/L
 4. cis-Aconitic acid 20mg/L

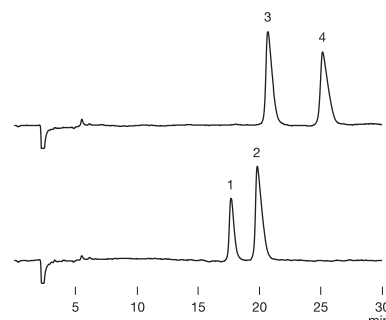

Column : Shodex IC SI-35 4D
Eluent : 9.0mM Na₂CO₃ aq.
Flow rate : 0.6mL/min
Detector : Suppressed conductivity
Column temp. : 45°C

Rapid analysis of anions using SI-35 2B (suppressor method)

Sample : 2μL
 1. F⁻ 1mg/L
 2. Cl⁻ 2mg/L
 3. NO₂⁻ 3mg/L
 4. Br⁻ 5mg/L
 5. NO₃⁻ 5mg/L
 6. PO₄³⁻ 8mg/L
 7. SO₄²⁻ 6mg/L

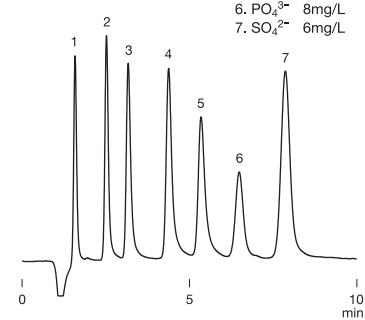

Column : Shodex IC SI-35 2B
Eluent : 1.0mM Na₂CO₃ + 2.0mM NaHCO₃ aq.
Flow rate : 0.2mL/min
Detector : Suppressed conductivity
Column temp. : 30°C

● Ion Chromatography Columns (Cation Analysis)

Features

- YS-50**
 - High performance type of YK-421
 - Applicable to both suppressor and non-suppressor methods
 - Provides sharp peaks; more significant for divalent cation analysis
 - Supports the analysis of alkylamines and transition metals

- YK-421**
 - Column for cation analysis with non-suppressor method
 - Simultaneous analysis of monovalent and divalent cations
 - Suitable separating of alkylamines
 - Fulfills USP L76 requirements

- Y-521**
 - Column for cation analysis with non-suppressor method
 - Separates monovalent cations or divalent cations
 - Fulfills USP L17 and L22 requirements

- T-521**
 - Column for transition metal ion analysis
 - Highly sensitive analysis achievable using post column color reaction method

■ Standard columns

[For cations]

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Base Material	Particle Size (μm)	Column Size (mm) I.D. x Length	Shipping Solvent
F7122000	IC YS-50	≥ 5,500	Carboxyl	Polyvinyl alcohol	5	4.6 × 125	H ₂ O
F6700530	IC YS-G	(guard column)	Carboxyl	Polyvinyl alcohol	5	4.6 × 10	H ₂ O
F7120012	IC YK-421	≥ 2,800	Carboxyl	Silica	5	4.6 × 125	5mM Tartaric acid + 1mM Dipicolinic acid + 1.5g/L Boric acid aq.
F6709608	IC YK-G	(guard column)	Carboxyl	Silica	5	4.6 × 10	5mM Tartaric acid + 1mM Dipicolinic acid + 1.5g/L Boric acid aq.
F6995210	IC Y-521	≥ 3,000	Sulfo	Styrene divinylbenzene copolymer	12	4.6 × 150	4mM HNO ₃ aq.
F6700230	IC Y-G	(guard column)	Sulfo	Styrene divinylbenzene copolymer	12	4.6 × 10	4mM HNO ₃ aq.

Housing Material: SUS

[For transition metal ions]

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (μm)	Column Size (mm) I.D. x Length	Shipping Solvent
F6995250	IC T-521	≥ 3,000	Sulfo	12	4.6 × 150	3mM HNO ₃ aq.
F6700412	IC T-G	(guard column)	Sulfo	12	4.6 × 10	3mM HNO ₃ aq.


Base Material: Styrene divinylbenzene copolymer
Housing Material: PEEK

■ Line filters for IC

Product Code	Product Name	Contents
F8500630	IC FL-1	One holder and one filter
F8500640	IC FL-1 filter	5 filters

Removes insoluble components in the eluent by installing it upstream of the injector

Common cations (YS-50 and YK-421)

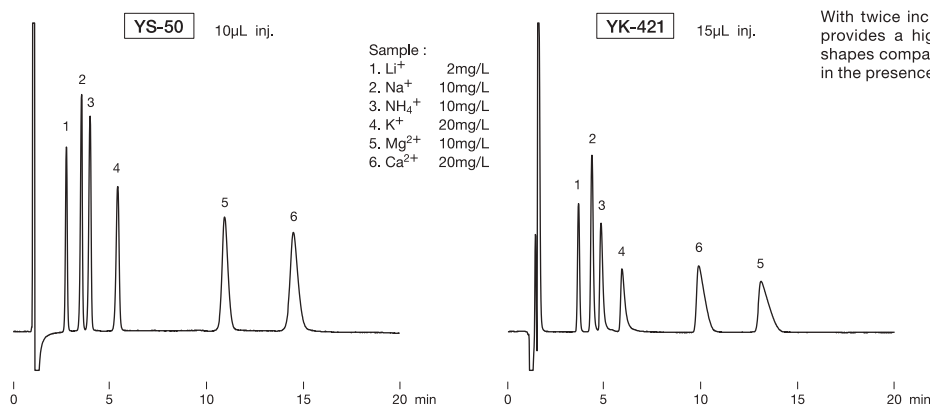

With twice increased theoretical plate number, YS-50 provides a higher performance with improved peak shapes compared to YK-421. The quantitation of NH_4^+ in the presence of high Na^+ content is also improved.

Resolution (Na^+ and NH_4^+)	YS-50	YK-421
	2.5	2.1


TP	YS-50	YK-421
Mg^{2+}	6,900	3,000
Ca^{2+}	6,600	3,000

Column : Shodex IC YS-50
Eluent : 4mM Methanesulfonic acid aq.
Flow rate : 1.0mL/min
Detector : Non-suppressed conductivity
Column temp. : 40°C

Column : Shodex IC YK-421
Eluent : 5mM Tartaric acid + 1mM Dipicolinic acid + 1.5g/L Boric acid aq.
Flow rate : 1.0mL/min
Detector : Non-suppressed conductivity
Column temp. : 40°C


Effects of added crown ether in the eluent

Crown ether forms complex with cations. The elution of cations (particularly K^+) can be well controlled by the difference in complex formation rate.

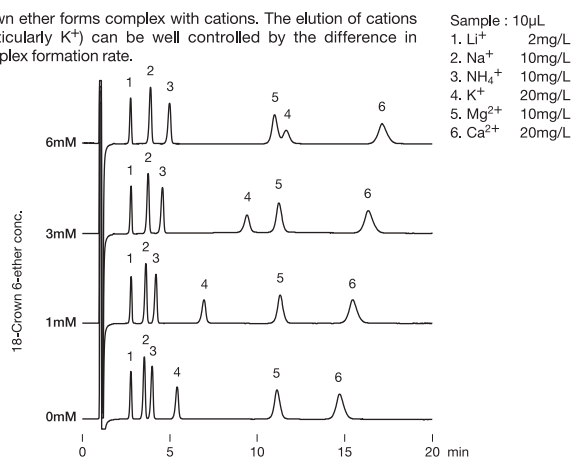


Column : Shodex IC YS-50
Eluent : 4mM Methanesulfonic acid + 18-Crown 6-ether aq.
Flow rate : 1.0mL/min
Detector : Non-suppressed conductivity
Column temp. : 40°C

Simultaneous analysis of cations and ethylenediamine

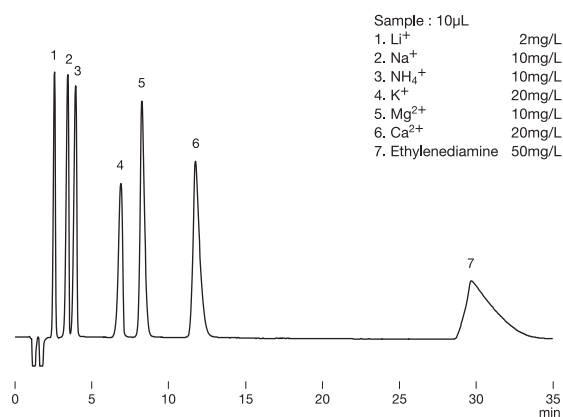


Column : Shodex IC YS-50
Eluent : 4mM HNO_3 + 1.5mM 18-Crown 6-ether aq.
Flow rate : 1.0mL/min
Detector : Non-suppressed conductivity
Column temp. : 40°C

Amino alcohols

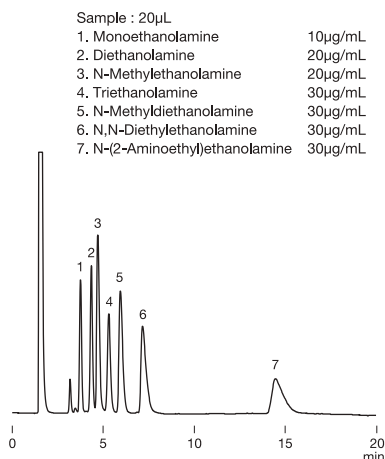


Column : Shodex IC YK-421
Eluent : 4mM HNO_3 aq.
Flow rate : 1.0mL/min
Detector : Non-suppressed conductivity
Column temp. : 40°C

Alkylamines

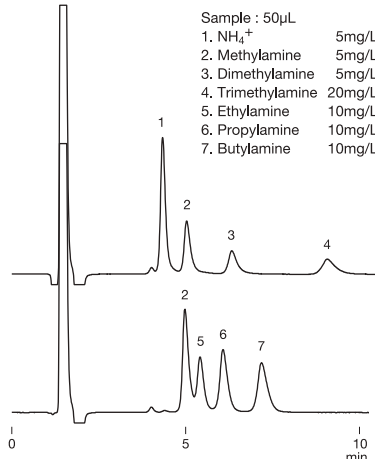

Column : Shodex IC YK-421
Eluent : 4mM H_3PO_4 aq./ CH_3CN =90/10
Flow rate : 1.0mL/min
Detector : Non-suppressed conductivity
Column temp. : 25°C

Alkaline earth metal ions

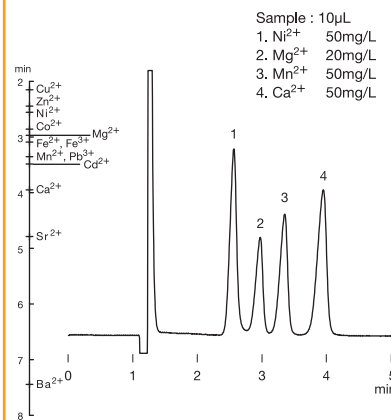


Column : Shodex IC Y-521
Eluent : 4mM Tartaric acid
+ 2mM Ethylenediamine aq.
Flow rate : 1.0mL/min
Detector : Non-suppressed conductivity
Column temp. : 40°C

Column Selection for Size Exclusion Chromatography (SEC)

	Application	Solvent	Column	Page
Aqueous SEC (GPC)	Biological macromolecules (proteins, peptides, nucleic acids, etc.)	Buffer etc.	KW-800 series	38
			LW-803 High performance	38
			KW400 series High performance (solvent-saving)	38
	Biological macromolecules (high MW range)	Buffer etc.	SB-800 HQ series	42
			LB-800 series	42
	Water-soluble polymers (polyacrylamide, polyethylenimine, etc.) Polysaccharides	Water, Buffer, Aqueous solution, etc.	SB-800 HQ series	42
			LB-800 series	42
	Oligosaccharide, polysaccharides	Water, Aqueous solution, etc.	KS-800 series	26
			GS-HQ series	46
Organic SEC (GPC)	General polymers	THF	KF-800 series	50
			KF-600 series Rapid analysis (solvent-saving)	56
			KF-400HQ series High performance (solvent-saving)	56
			HK-400 series Ultra-rapid Analysis (solvent-saving)	58
			LF series High-linear calibration curves	62
	Polar polymers (polyimides, polyvinylpyrrolidones etc.)	Chloroform	K-800 series	52
			KD-800 series	54
			HK-400 series Ultra-rapid Analysis (solvent-saving)	58
			LF series High-linear calibration curves	62
			SB-800 HQ series	42
	Analysis at high temperature (polyethylene, polypropylene etc.)	DMF	LB-800 series	42
			HT-800 series	64
			UT-800 series	64
	Engineering resin analysis at room temperature [polyamide (Nylon), polyethylene terephthalate (PET) etc.]	ODCB etc.	AT-806MS	64
			HFIP-800 series	66
			HFIP-600 series Rapid analysis (solvent-saving)	66
			HK-HFIP404L Ultra-rapid Analysis (solvent-saving)	58
		HFIP	LF series High-linear calibration curves	62
Aqueous/Organic SEC			GF-HQ series	48

Solvent usability guideline for the Shodex SEC columns

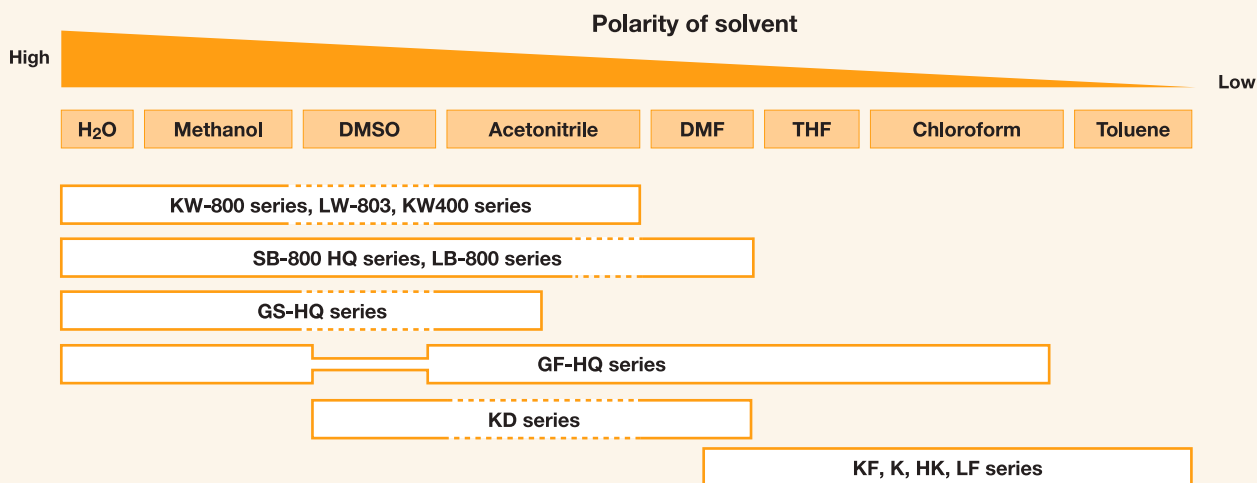

*See page 68 for the solvent replaceability of organic solvent SEC (GPC) packed columns.

● Precautions for Polar Polymer Analysis

Unexpected interactions in the column can affect the size exclusion chromatography analysis of polar polymers. These interactions may change elution patterns and results in an invalid molecular weight calculation. It is important to reduce these interfering interactions in order to obtain the accurate molecular weight distribution.

Interfering interactions likely to be observed

Interactions between the analyte and the packing materials


- **Hydrophobic interaction**
 - The analyte is adsorbed on the packing material. This delays the analyte elution and results in under estimating the analyte's molecular weight. See (B) and (D).
- **Ionic interaction**
 - (1) Ion Exclusion
 - The analyte is repelled from the packing material. This accelerates the analyte elution and results in over estimating the analyte's molecular weight. See (A) and (C).
 - (2) Ion Exchange
 - The analyte is adsorbed on the packing material. This delays the analyte elution and results in under estimating the analyte's molecular weight. See (B) and (D).

Interaction within and between the analyte

- **Ionic repulsion effects observed within the multivalent macromolecules causes structure expansion**
 - This accelerates the analyte elution and results in over estimating the analyte's molecular weight. See (A).
- **Association between the molecules**
 - This accelerates the analyte elution and results in over estimating the analyte's molecular weight. See (A).

Interactions between the analyte and the solvent

- **The multivalent ion in the solvent works as a bridge to bind ionic molecules (analyte).**

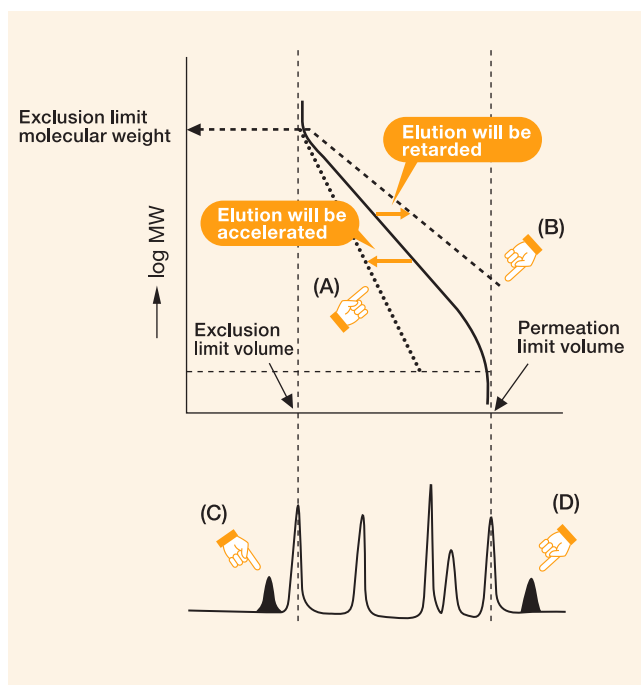

Methods to reduce interactions

Aqueous SEC (GFC)

Ionic Interaction

- Add salt

Hydrophobic interaction

- **Increase the analyte dissociation**
Cationic polymer → Lower the pH
Anionic polymer → Higher the pH
- **Lower the eluent polarity**
(Example) Add acetonitrile or methanol

Organic solvent SEC (GPC)

Ionic Interaction

- Add salt
(Example) Add LiBr to DMF
Add CF₃COONa to HFIP

Hydrophobic interaction

- **Lower the eluent polarity**
(Example) Change the eluent from DMF to THF

Hydrophillic interaction

- **Increase the eluent polarity**
(Example) Change the eluent from THF to DMF

● Aqueous SEC (GFC) Columns: Silica-based

Features

KW-800

- Silica-based packed columns for aqueous SEC (GFC) analysis
- Suitable for the analysis of proteins and enzymes
- Fulfills USP L20, L33, and L59 requirements

New LW-803

- Suitable for pore size specifically controlled for analyzing proteins with molecular weights of several hundred thousand
- High performance analysis of antibody drugs and various proteins
- High lot-to-lot reproducibility
- Fulfills USP L20, L33, and L59 requirements

KW400

- Reduced packing material particle size enhances column performance
- Three to four-fold higher sensitivity than KW-800 series
- KW405-4F is applicable analyzing samples with molecular weight above 1,000,000
- Fulfills USP L20, L33, and L59 requirements

■ Standard columns

Product Code	Product Name	¹⁾ Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6989000	PROTEIN KW-802.5	≥ 21,000	5	400	8.0 × 300	H ₂ O
F6989103	PROTEIN KW-803	≥ 21,000	5	1,000	8.0 × 300	H ₂ O
F6989104	PROTEIN KW-804	≥ 16,000	7	1,500	8.0 × 300	H ₂ O
F6700131	PROTEIN KW-G 6B (PROTEIN KW-G)	(guard column)	7	–	6.0 × 50	H ₂ O

1) Measured with ethylene glycol

Base Material: Silica

Usable pH range: pH3.0-7.5

Usable concentration of methanol and acetonitrile is up to 100%

■ Standard columns

Product Code	Product Name	²⁾ Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6989303	New PROTEIN LW-803	≥ 12,000	3	1,000	8.0 × 300	H ₂ O
F6700133	New PROTEIN LW-G 6B	(guard column)	3	–	6.0 × 50	H ₂ O

2) Measured with BSA

Base Material: Silica

Usable pH range: pH3.0-7.5

Usable concentration of methanol and acetonitrile is up to 100%

■ High performance semi-micro columns

© KW400 series is recommended to be used with semi-micro type devices.

Product Code	Product Name	³⁾ Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6989201	KW402.5-4F	≥ 35,000	3	400	4.6 × 300	H ₂ O
F6989202	KW403-4F	≥ 35,000	3	800	4.6 × 300	H ₂ O
F6989203	KW404-4F	≥ 25,000	5	1,500	4.6 × 300	H ₂ O
F6989204	KW405-4F	≥ 25,000	5	2,000	4.6 × 300	H ₂ O
F6700132	KW400G-4A	(guard column)	5	–	4.6 × 10	H ₂ O

3) Measured with uridine

Base Material: Silica

Usable pH range: pH3.0-7.5

Usable concentration of methanol and acetonitrile is up to 100%

Preparative columns *Preparative columns are made to order.

Product Code	Product Name	4) Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6505020	PROTEIN KW-2002.5	≥ 17,000	5	20.0 × 300	KW-802.5
F6505021	PROTEIN KW-2003	≥ 17,000	5	20.0 × 300	KW-803
F6505022	PROTEIN KW-2004	≥ 14,000	7	20.0 × 300	KW-804
F6709556	PROTEIN KW-G 8B (PROTEIN KW-LG)	(guard column)	7	8.0 × 50	(guard column)

4) Measured with ethylene glycol

Target molecular weight range and exclusion limit

Measured with protein (eluent: phosphate buffer)

Product Name	Target Molecular Weight Range	Exclusion Limit
KW-802.5	5,000 – 100,000	150,000
KW-803, LW-803	10,000 – 700,000	*(1,000,000)
KW-804	30,000 – *(4,000,000)	*(4,000,000)
KW402.5	5,000 – 70,000	150,000
KW403	10,000 – 500,000	600,000
KW404	30,000 – *(4,000,000)	*(4,000,000)
KW405	200,000 – *(20,000,000)	*(20,000,000)

*Please use the above table for reference purposes only when selecting columns.


*() Estimated value

Measured with pullulan (eluent: ultrapure water)

Product Name	Target Molecular Weight Range	Exclusion Limit
KW-802.5	2,000 – 50,000	60,000
KW-803	5,000 – 100,000	170,000
KW-804	20,000 – 300,000	500,000
KW402.5	2,000 – 40,000	60,000
KW403	3,000 – 50,000	80,000
KW404	20,000 – 300,000	400,000
KW405	100,000 – 700,000	1,300,000


*Please use the above table for reference purposes only when selecting columns.

Calibration curves for KW-800 series using protein

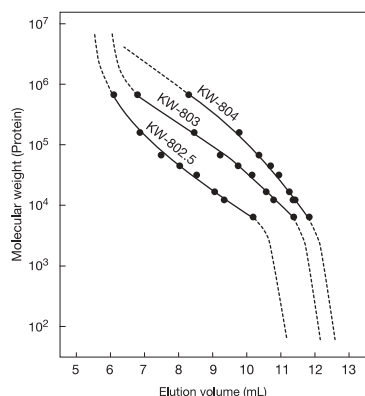


Column : Shodex PROTEIN KW-800 series
Eluent : 50mM Sodium phosphate buffer (pH7.0) + 0.3M NaCl
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : 30°C

Calibration curve for LW-803 using protein

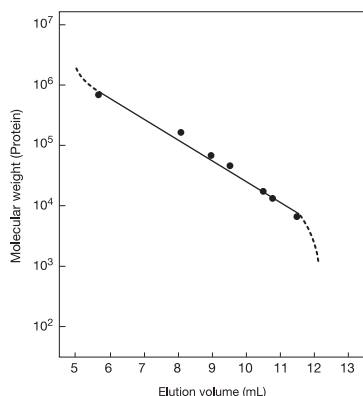

Column : Shodex PROTEIN LW-803
Eluent : 50mM Sodium phosphate buffer (pH7.0) + 0.3M NaCl
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : Room temp.


Calibration curves for KW400 series using protein

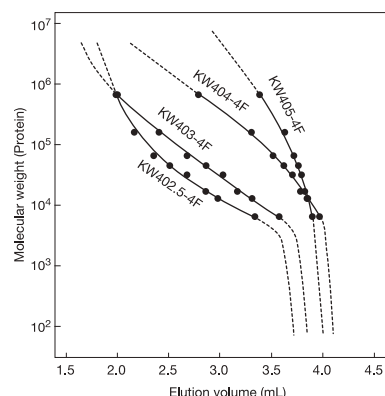

Column : Shodex KW400-4F series
Eluent : 50mM Sodium phosphate buffer (pH7.0) + 0.3M NaCl
Flow rate : 0.33mL/min
Detector : UV (280nm) (small cell volume)
Column temp. : 30°C

Analysis of impurities (high molecular weight proteins) in insulin glargine following USP method


Sample : 100μL
 System suitability solution
 (prepared following USP method)
 1. High molecular weight proteins
 2. Insulin glargine

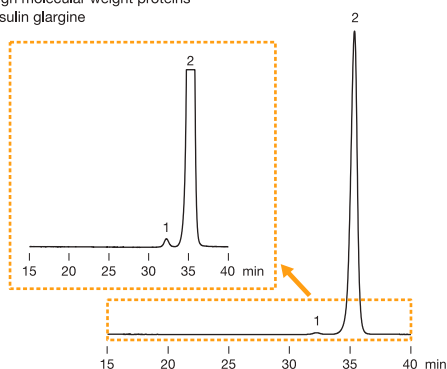

Column : Shodex PROTEIN KW-802.5 x 2
Eluent : CH₃COOH/CH₃CN/H₂O=20/30/50 (pH to 3.0 adjusted with 25% NH₃ aq.)
Flow rate : 0.5mL/min
Detector : UV (276nm)
Column temp. : Ambient

Lipoproteins in serum

Sample : 40μL
 Whole lipoproteins from serum
 of a healthy person 1.0mg/mL
 1. VLDL
 2. LDL
 3. HDL

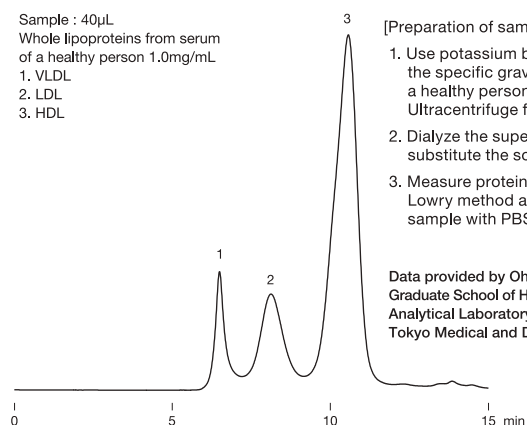

[Preparation of sample]


1. Use potassium bromide to adjust the specific gravity of serum from a healthy person to 1.210g/mL. Ultracentrifuge for 24 hours.
2. Dialyze the supernatant and then substitute the solvent with PBS*.
3. Measure protein concentration by Lowry method and dilute the sample with PBS* to 1.0mg/mL.

Data provided by Ohkawa Ryunosuke, Graduate School of Health Care Sciences, Analytical Laboratory Chemistry, Tokyo Medical and Dental University

Column : Shodex PROTEIN KW-G + KW-804
Eluent : 10-fold diluted x 10 PBS* with H₂O
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : 30°C

x10 PBS* : 80g NaCl + 29g Na₂HPO₄ · 12H₂O + 2g KCl + 2g KH₂PO₄ in 1000mL of H₂O

Proteins in human blood serum

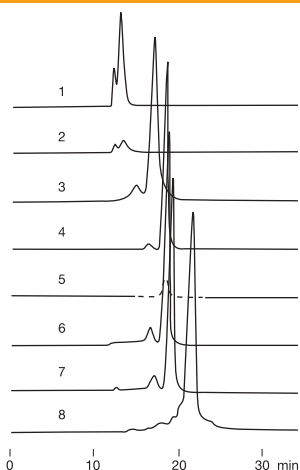


Sample : 0.1% each
 1. Fibrinogen 50μL
 2. α₂-Macroglobulin 50μL
 3. IgG 50μL
 4. Transferrin 50μL
 5. Plasminogen 50μL
 6. Albumin 100μL
 7. Antitrypsin 100μL
 8. Hemoglobin 100μL


Column : Shodex PROTEIN KW-803
Eluent : 50mM Sodium phosphate buffer (pH7.0) + 0.3M NaCl
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : Room temp.

Comparing three GFC columns for the separation of common proteins

Sample :
 1. Thyroglobulin (bovine)
 2. γ-Globulin (bovine)
 3. Ovalbumin (chicken)
 4. Myoglobin (horse)
 5. Cyanocobalamin

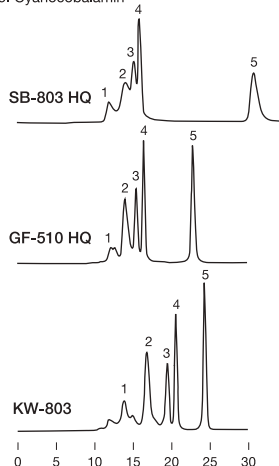

Separation performances of three aqueous SEC columns (SB-803 HQ, GF-510 HQ, and KW-803) were compared. KW-803, silica-based column, showed the best separation performance for the analysis of protein standards.

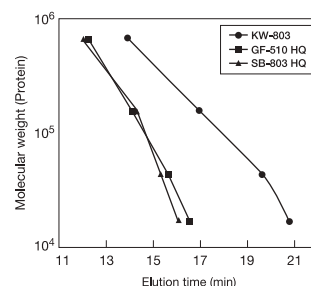


Column : Shodex OHpak SB-803 HQ
 Shodex Asahipak GF-510 HQ
 Shodex PROTEIN KW-803
Eluent : 0.2M Phosphate buffer (pH6.9)
Flow rate : 0.5mL/min
Detector : UV (280nm)
Column temp. : 30°C

Comparison of LW-803, conventional column, and other manufacturer's column


PROTEIN LW-803 is suitable for analyzing proteins with molecular weight of several hundreds of thousands. Compared to our conventional columns and other manufacturer's columns, LW-803 has improved separation performance in the molecular weight range around 160,000 (about the size of γ -Globulin). This improvement is advantageous for the separation of monomer and dimer of IgG which is a mainstream antibody drug.

Sample : 5 μ L
 1. Thyroglobulin (MW : 670,000) 7mg/mL
 2. γ -Globulin (MW : 160,000) 6mg/mL
 3. Ovalbumin (MW : 44,300) 4.8mg/mL
 4. Ribonuclease A (MW : 13,700) 7mg/mL
 5. Uridine (MW : 244) 0.1mg/mL


LW-803

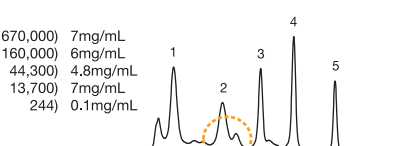

(conventional type)
KW-803




Company A

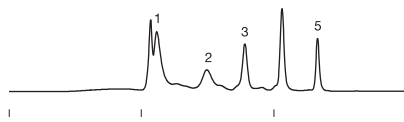


Sample : 5 μ L
 IgG from human serum 10mg/mL
 1. Aggregates
 2. Dimer
 3. Monomer


LW-803

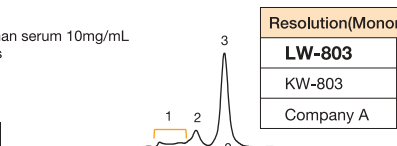

(conventional type)
KW-803




Company A

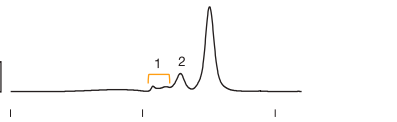

Resolution(Monomer/Dimer)	
LW-803	2.2
KW-803	1.6
Company A	1.9

Column : Shodex PROTEIN LW-803, Shodex PROTEIN KW-803, Silica-based SEC column from other manufacturer
 Eluent : 50mM Sodium phosphate buffer (pH7.0) + 0.3M NaCl
 Flow rate : 1.0mL/min
 Detector : UV (280nm)
 Column temp. : Room temp.

Monitoring papain digestion of humanized monoclonal IgG

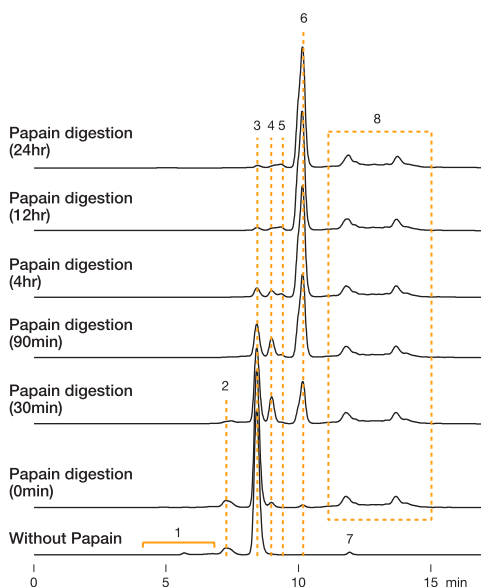

Sample : 10 μ L
 Humanized monoclonal IgG
 1. Aggregates of IgG
 2. Dimer of IgG
 3. Monomer of IgG
 4, 5, 6. Fragments of IgG from papain digestion
 7. Citric acid
 8. Papain

Papain digestion of humanized monoclonal IgG was monitored using PROTEIN LW-803, an aqueous SEC (GFC) column. During the papain digestion of IgG, Fc and Fab fragments from the IgG and their decomposition intermediates are expected to be observed. LW-803 separates IgG and decomposed fragments and intermediates well from each other, thus it is suitable for the monitoring of papain digestion of IgG.

[Procedure of papain digestion]


- (1) Dissolve 3mg of humanized monoclonal IgG in 500 μ L of the eluent. (6mg/mL conc.)
- (2) Dissolve 1mg of papain in 500 μ L of the eluent. (1mg/mL conc.)
- (3) Pass (1) and (2) through 0.2 μ m membrane filter.
- (4) Mix each solution in equal amounts.
- (5) Keep temperature at 25°C.
- (6) Takes a sample with time and analyze it by HPLC.

Column : Shodex PROTEIN LW-803
 Eluent : 0.1M Sodium phosphate buffer (pH7.0) + 0.3M NaCl
 Flow rate : 1.0mL/min
 Detector : UV (280nm)
 Column temp. : 25°C

Comparison of KW402.5-4F and KW-802.5

KW400 series is a high performance type of semi-micro columns. It offers approximately 1.5 times larger theoretical plate number and 3 to 4 times higher detection sensitivity (peak height) than KW-800 series columns do.


Sample : 10 μ L
 1. Blue dextran 2000 0.2mg/mL
 2. γ -Globulin 0.8mg/mL
 3. Ovalbumin 0.8mg/mL
 4. Myoglobin 0.56mg/mL
 5. Uridine 0.04mg/mL

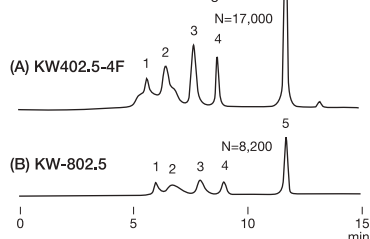

Column : Shodex KW402.5-4F
 Shodex PROTEIN KW-802.5
 Eluent : 50mM Sodium phosphate buffer (pH7.0) + 0.3M NaCl
 Flow rate : (A) 0.33mL/min, (B) 1.0mL/min
 Detector : UV (280nm) (small cell volume)
 Column temp. : 25°C

Whey in yogurt


Sample : Whey, 5 μ L

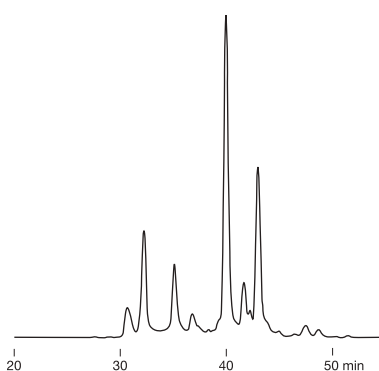

Column : Shodex KW402.5-4F + KW403-4F
 Eluent : 50mM Sodium phosphate buffer (pH7.0) + 0.3M NaCl
 Flow rate : 0.20mL/min
 Detector : UV (280nm) (small cell volume)
 Column temp. : 30°C

Lectins

Sample : 5 μ L
 1. Lectin from soybean 0.6mg/mL
 2. Lectin from arachis hypogaea 1.1mg/mL
 3. Lectin from canavalia ensiformis (Con A) 0.9mg/mL
 4. Lectin from lens culinaris (LCA) 0.7mg/mL
 5. Lectin from triticum vulgaris (WGA) 0.8mg/mL

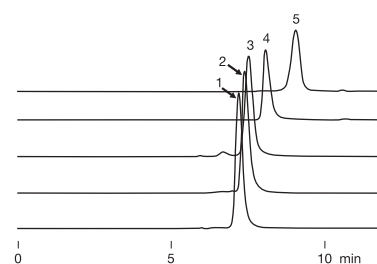

Column : Shodex KW402.5-4F
 Eluent : 50mM Sodium phosphate buffer (pH7.0) + 0.3M NaCl
 Flow rate : 0.33mL/min
 Detector : UV (220nm) (small cell volume)
 Column temp. : 30°C

● Aqueous SEC (GFC) Columns: Polymer-based

Features

- SB-800 HQ**
- Polymer-based packed columns for aqueous SEC (GFC) analysis
 - Supports a wide range of molecular weight sample analysis
 - The eluent can be replaced with DMF (except SB-802 HQ and SB-807 HQ), enabling the analysis of polar polymers
 - Method using SB-804 HQ or SB-805 HQ for gelatin's mean molecular weight determination is comparable with PAGI method (Ver. 10, Japan)
 - Fulfills USP L38 and L39 requirements
 - SB-802 and 802.5 HQ fulfill USP L25 requirements
 - SB-803 HQ fulfills USP L37 requirements
- SB-807 HQ**
- Column for the analysis of water-soluble ultra high molecular weight polymers
 - Large particle-size gel prevents shear degradation of polymers
 - Fulfills USP L38 and L39 requirements
- LB-800**
- Polymer-based packed columns for aqueous SEC (GFC) analysis
 - Controlled column bleeding allows its use with light scattering detectors
 - The eluent can be replaced with DMF enabling the analysis of polar polymers
 - LB-805 (exclusion limit: about 4,000,000) newly added to the series
 - Fulfills USP L38 and L39 requirements

■ Standard columns

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6429100	OHpak SB-802 HQ	≥ 12,000	8	100	8.0 × 300	0.02% NaN ₃ aq.
F6429101	OHpak SB-802.5 HQ	≥ 16,000	6	200	8.0 × 300	0.02% NaN ₃ aq.
F6429102	OHpak SB-803 HQ	≥ 16,000	6	800	8.0 × 300	0.02% NaN ₃ aq.
F6429103	OHpak SB-804 HQ	≥ 16,000	10	2,000	8.0 × 300	0.02% NaN ₃ aq.
F6429104	OHpak SB-805 HQ	≥ 12,000	13	7,000	8.0 × 300	0.02% NaN ₃ aq.
F6429105	OHpak SB-806 HQ	≥ 12,000	13	15,000	8.0 × 300	0.02% NaN ₃ aq.
F6429106	OHpak SB-806M HQ	≥ 12,000	13	15,000	8.0 × 300	0.02% NaN ₃ aq.
F6709430	OHpak SB-G 6B (OHpak SB-G)	(guard column)	10	–	6.0 × 50	0.02% NaN ₃ aq.

SB-806M HQ is a mixed-gel column capable of analyzing samples over a wide range of molecular weight distribution.

Base Material: Polyhydroxymethacrylate
Usable pH range: pH3-10

[Aqueous high molecular weight analysis column]

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6429108	OHpak SB-807 HQ	≥ 1,500	35	30,000	8.0 × 300	H ₂ O
F6709431	OHpak SB-807G	(guard column)	35	–	8.0 × 50	H ₂ O

Base Material: Polyhydroxymethacrylate
Usable pH range: pH3-10

[GFC columns to be used with light scattering detector]

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6429201	OHpak LB-803	≥ 16,000	6	800	8.0 × 300	H ₂ O
F6429203	New OHpak LB-805	≥ 12,000	13	7,000	8.0 × 300	H ₂ O
F6429202	OHpak LB-806M	≥ 12,000	13	15,000	8.0 × 300	H ₂ O
F6709434	OHpak LB-G 6B	(guard column)	13	–	6.0 × 50	H ₂ O

Base Material: Polyhydroxymethacrylate
Usable pH range: pH3-10

Preparative columns *Preparative columns are made to order.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6516011	OHpak SB-2002	≥ 9,000	15	20.0 × 300	SB-802 HQ
F6516012	OHpak SB-2002.5	≥ 12,000	10	20.0 × 300	SB-802.5 HQ
F6516013	OHpak SB-2003	≥ 12,000	10	20.0 × 300	SB-803 HQ
F6516014	OHpak SB-2004	≥ 12,000	18	20.0 × 300	SB-804 HQ
F6516015	OHpak SB-2005	≥ 12,000	20	20.0 × 300	SB-805 HQ
F6516016	OHpak SB-2006	≥ 12,000	20	20.0 × 300	SB-806 HQ
F6516017	OHpak SB-2006M	≥ 12,000	20	20.0 × 300	SB-806M HQ
F6709555	OHpak SB-G 8B (OHpak SB-LG)	(guard column)	18	8.0 × 50	(guard column)

Usable concentration of organic solvents

Product Code	The maximum usable concentration (%)		
	Methanol	Acetonitrile	DMF
SB-802 HQ	0	0	0
SB-802.5 HQ, SB-803 HQ	100	75	100
SB-804 HQ~SB-806M HQ	75	75	100
SB-G 6B	75	75	100
SB-807 HQ, SB-807G	30	30	0
LB-803, LB-805, LB-806M, LB-G 6B	100	100	100

(Note)
The maximum solvent tolerance of SB-2000 series, preparative columns of SB-800 series, is 50% methanol, acetonitrile, or DMF (SB-2002 is not tolerant to organic solvents).

Target molecular weight range and exclusion limit

Measured with pullulan (eluent: ultrapure water)

Product Name	Target Molecular Weight Range	Exclusion Limit
SB-802 HQ	200 – 1,000	1,000
SB-802.5 HQ	500 – 10,000	10,000
SB-803 HQ	1,000 – 100,000	100,000
SB-804 HQ	5,000 – 400,000	1,000,000
SB-805 HQ	100,000 – 1,000,000	*(4,000,000)
SB-806 HQ	100,000 – *(20,000,000)	*(20,000,000)
SB-806M HQ	500 – *(20,000,000)	*(20,000,000)
SB-807 HQ	500,000 – *(500,000,000)	*(500,000,000)
LB-803	1,000 – 100,000	100,000
LB-805	100,000 – 1,000,000	*(4,000,000)
LB-806M	500 – *(20,000,000)	*(20,000,000)

*Please use the above table for reference purposes only when selecting columns.

*() Estimated value


Measured with *PEG/PEO (eluent: DMF)

Product Name	Target Molecular Weight Range
SB-802.5 HQ	100 – 2,000
SB-803 HQ	200 – 40,000
SB-804 HQ	500 – 300,000
SB-805 HQ	50,000 – 700,000
SB-806 HQ	70,000 – *(20,000,000)
SB-806M HQ	200 – *(20,000,000)
LB-803	500 – 50,000
LB-805	50,000 – 700,000
LB-806M	200 – *(20,000,000)

*Please use the above table for reference purposes only when selecting columns.


*PEG: polyethylene glycol
*PEO: polyethylene oxide
** () Estimated value

Calibration curves for SB-800 HQ series using pullulan (eluent: H₂O)

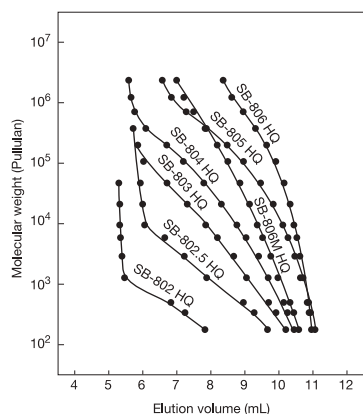

Column : Shodex OHpak SB-800 HQ series
Eluent : H₂O
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 30°C


Calibration curves for SB-800 HQ series using PEG/PEO (eluent: DMF)

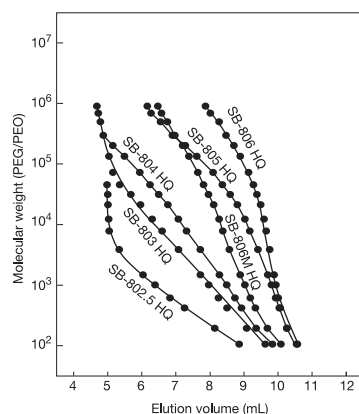

Column : Shodex OHpak SB-800 HQ series
Eluent : DMF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Carboxymethylcellulose

Sample : Carboxymethylcellulose 0.1% each, 50μL

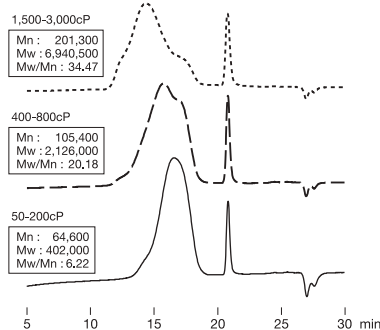


*Molecular weight was determined from the calibration curve of pullulan.

Column : Shodex OHpak SB-806M HQ x 2
Eluent : 0.1M NaCl aq.
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Effects of sodium nitrate in eluent on the analysis of polyallylamine

For the analysis of cationic polymers, such as polyallylamine, undesired adsorption of the polymer is observed when low (0.02M) sodium nitrate eluent was used. By using higher concentration (> 0.1M) salt, it suppresses the sample adsorption and enables to obtain accurate chromatograms.


Sample : Polyallylamine 0.2%, 100μL

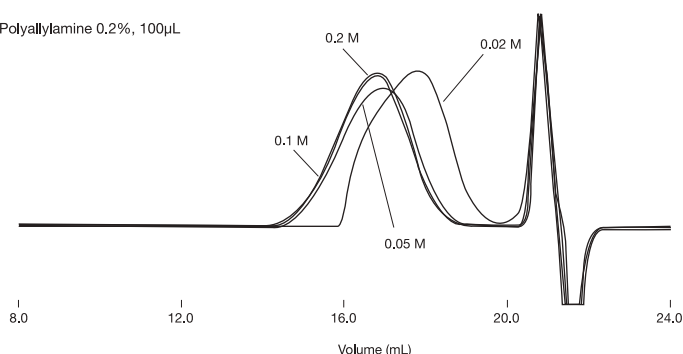

Column : Shodex OHpak SB-806M HQ x 2
Eluent : 0.5M CH₃COOH + NaNO₃ aq.
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Gelatin


Sample : 0.1% each, 100μL
 Gelatin from bovine skin
 (Acid treatment, Gel strength : 225g)
 Gelatin from porcine skin
 (Alkali treatment, Gel strength : 90-100g)

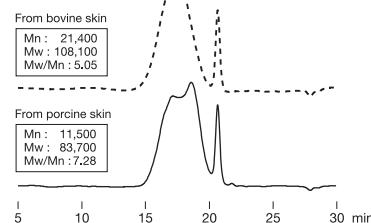

*Molecular weight was determined from the calibration curve of pullulan.

Column : Shodex OHpak SB-806M HQ x 2
Eluent : 0.1M KH₂PO₄ aq./
 0.1M Na₂HPO₄ aq.=50/50
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C


Polyacrylamide

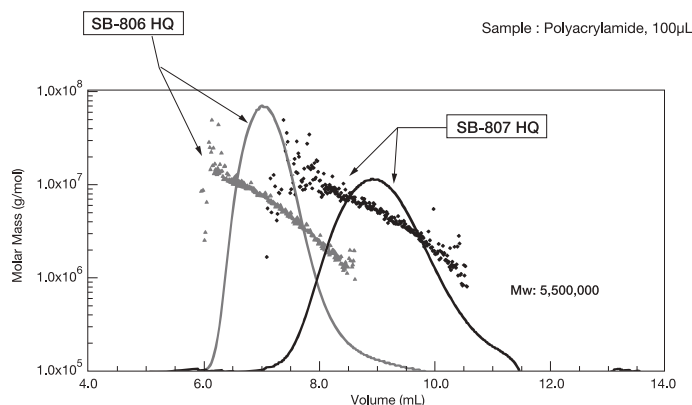

Column : Shodex OHpak SB-807 HQ, SB-806 HQ
Eluent : 0.2M NaCl aq.
Flow rate : 0.5mL/min
Detector : RI
 MALS (Multi angle light scattering)
Column temp. : 30°C

Cellulose acetate

Sample : Cellulose acetate 0.1% each, 100μL

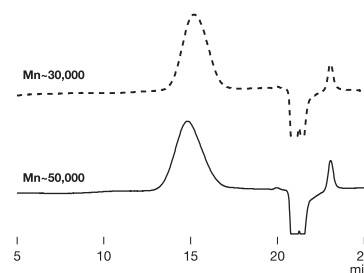

Column : Shodex OHpak SB-806M HQ x 2
Eluent : 20mM LiBr in DMF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Copovidones

Sample : 100 μ L
Poly(1-vinylpyrrolidone-co-vinyl acetate) 0.1% each


Copolymer 7:3
Mn : 2,000
Mw : 14,400
Mw/Mn : 7.40

Copolymer 3:7
Mn : 6,400
Mw : 28,900
Mw/Mn : 4.53

*Molecular weight was determined from the calibration curve of PEG/PEO.


Column : Shodex OHpak SB-806M HQ x 2
Eluent : 20mM LiBr in DMF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Calibration curves for LB-800 series using pullulan (eluent: H₂O)

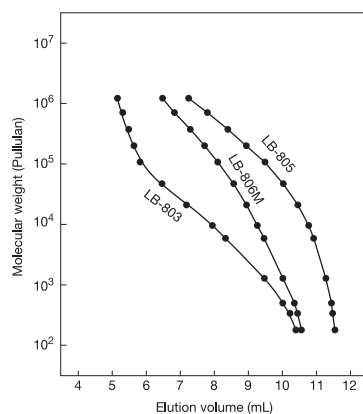

Column : Shodex OHpak LB-800 series
Eluent : H₂O
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 30°C



Calibration curves for LB-800 series using PEG/PEO (eluent: DMF)

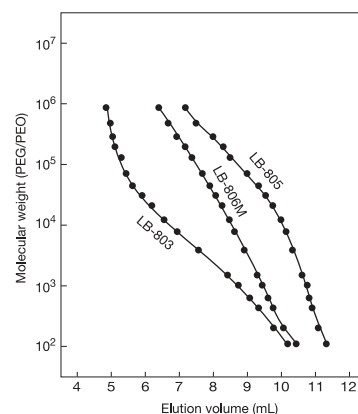

Column : Shodex OHpak LB-800 series
Eluent : DMF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Pullulan detection by LB-806M and multiangle light scattering detector


The new OHpak LB-800 series is able to detect low molecular weight substances owing to its improved low baseline noise level while using it with a multiangle light scattering detector. This cannot be achieved with other manufacturer's SEC column.

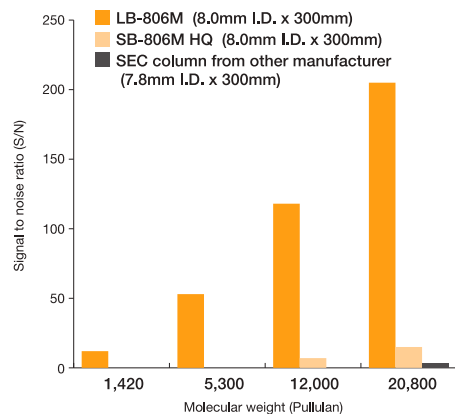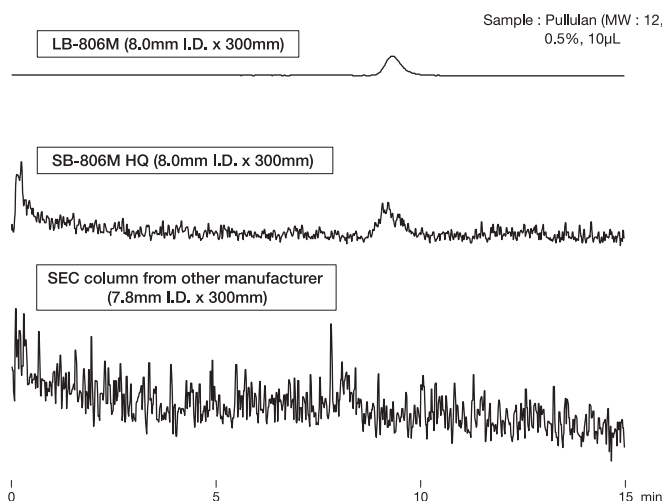

Column : Shodex OHpak LB-806M
Shodex OHpak SB-806M HQ
SEC column from other manufacturer
Eluent : 0.1M NaNO₃ aq.
Flow rate : 1.0mL/min
Detector : MALS (Multi angle light scattering) (90°)
Column temp. : 30°C

Sodium alginate


Sample : Sodium alginate 0.1%, 100 μ L

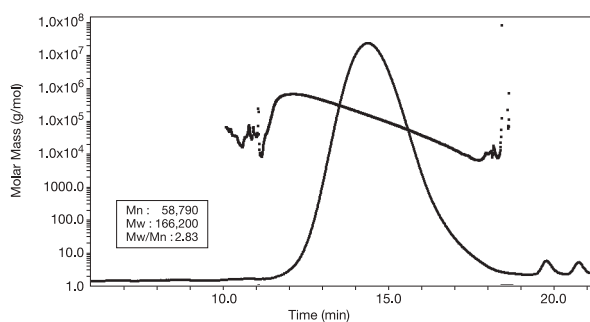

Column : Shodex OHpak LB-806M x 2
Eluent : 0.1M NaNO₃ aq.
Flow rate : 1.0mL/min
Detector : RI
MALS (Multi angle light scattering)
Column temp. : 30°C

Sodium heparin

Sample : Sodium heparin 0.1%, 100 μ L

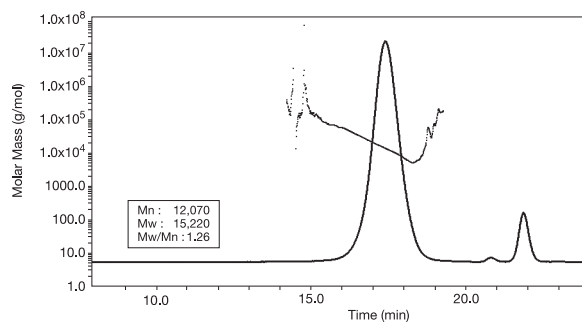

Column : Shodex OHpak LB-806M x 2
Eluent : 0.1M NaNO₃ aq.
Flow rate : 1.0mL/min
Detector : RI
MALS (Multi angle light scattering)
Column temp. : 30°C

Multimode Columns

Features

- GS-HQ**
- SEC is the main separation mode
 - With the choice of eluent, the column provides multimode features of reversed phase, HILIC, and ion exchange modes to SEC
 - Suitable for the separation of peptides or nucleic acids with similar molecular weights
 - Suitable for desalting samples or substituting buffer in protein analysis

Standard columns

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7600005	Asahipak GS-220 HQ	≥ 19,000	6	150	7.5 × 300	H ₂ O/CH ₃ OH=70/30
F7600006	Asahipak GS-320 HQ	≥ 19,000	6	400	7.5 × 300	H ₂ O/CH ₃ OH=70/30
F7600007	Asahipak GS-520 HQ	≥ 18,000	7	2,000	7.5 × 300	H ₂ O/CH ₃ OH=70/30
F7600008	Asahipak GS-620 HQ	≥ 18,000	7	7,000	7.5 × 300	H ₂ O/CH ₃ OH=70/30
F6710019	Asahipak GS-2G 7B	(guard column)	9	–	7.5 × 50	H ₂ O/CH ₃ OH=70/30

Base Material: Polyvinyl alcohol
 Usable pH range: pH2-12 (GS-220 HQ: pH2-9)
 Usable concentration of methanol is up to 100% (GS-220 HQ: up to 30%)
 Usable concentration of acetonitrile is up to 50%

Semi-micro columns

***The following semi-micro columns are made to order.**

Product Code	Product Name	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F7750312	GS320A-4D	6	400	4.6 × 150
F7750311	GS320A-4E	6	400	4.6 × 250

Base Material: Polyvinyl alcohol

Preparative columns *Preparative columns are made to order.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6810017	Asahipak GS-220 20F	≥ 8,000	13	20.0 × 300	GS-220 HQ
F6810018	Asahipak GS-320 20F	≥ 8,000	13	20.0 × 300	GS-320 HQ
F6810019	Asahipak GS-520 20F	≥ 8,000	13	20.0 × 300	GS-520 HQ
F6810020	Asahipak GS-620 20F	≥ 8,000	13	20.0 × 300	GS-620 HQ
F6810034	Asahipak GS-220 20G	≥ 14,000	13	20.0 × 500	GS-220 HQ
F6810035	Asahipak GS-320 20G	≥ 14,000	13	20.0 × 500	GS-320 HQ
F6810036	Asahipak GS-520 20G	≥ 14,000	13	20.0 × 500	GS-520 HQ
F6810037	Asahipak GS-620 20G	≥ 14,000	13	20.0 × 500	GS-620 HQ
F6710021	Asahipak GS-20G 7B	(guard column)	20	7.5 × 50	(guard column)


Target molecular weight range and exclusion limit

● Measured with pullulan (eluent: ultrapure water)

Product Name	Target Molecular Weight Range	Exclusion Limit
GS-220	300 – 3,000	7,000
GS-320	300 – 20,000	40,000
GS-520	5,000 – 200,000	300,000
GS-620	10,000 – 800,000	1,000,000

*Please use the above table for reference purposes only when selecting columns.

Calibration curves for GS-HQ series using pullulan

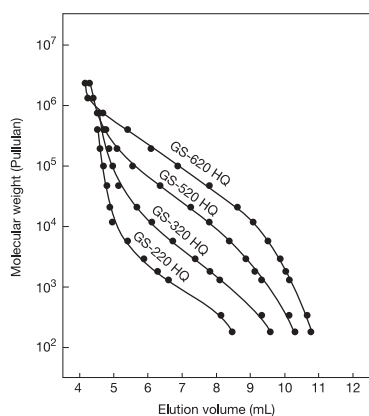

Column : Shodex Asahipak GS-HQ series
Eluent : H₂O
Flow rate : 0.6mL/min
Detector : RI
Column temp. : 30°C

Peptides


GS-HQ columns work not only under SEC (GFC) mode, but also under multimode, adding hydrophobic and ionic interactions. By carefully selecting the eluent, they provide separation mode that was not available with other types of columns. GS-320 HQ shows excellent performance separating hydrophilic peptides, particularly for acidic and basic peptides.

	MW	pI	Σf
Glu-Ala-Glu	347	3.12	0.39
Arg-Asp	289	6.75	0.68
Gly-His-Lys	340	9.95	0.29
Arg-Pro-Lys-Pro	497	11.44	3.24

Σf: Hydrophobic parameter
 pI: Isoelectric point

Column : Shodex Asahipak GS-320 HQ
Eluent : 30mM Ammonium acetate buffer (pH6.7)
Flow rate : 0.5mL/min
Detector : UV (220nm)
Column temp. : 30°C


Sample : 20μL
 1. Glu-Ala-Glu 0.025%
 2. Arg-Asp 0.05%
 3. Gly-His-Lys 0.025%
 4. Arg-Pro-Lys-Pro 0.025%

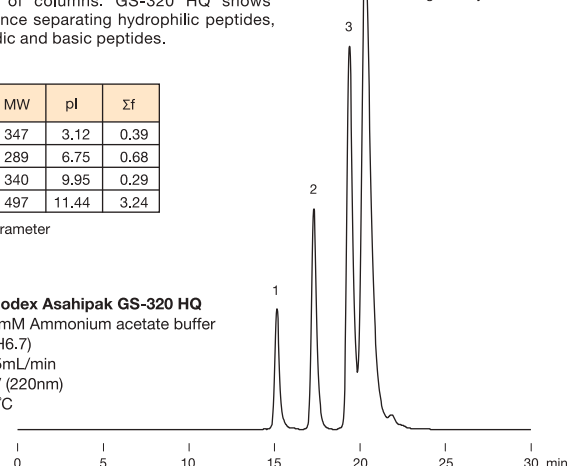


Analysis of purine bases in beer

Purine in food is analyzed as purine base after steps of sample preparation: homogenization, freeze drying, hydrolyzation with 70% perchloric acid, and neutralization. Example below shows the analysis of purine in regular beer and beer treated with guanase (an enzyme that degrades guanine to xanthine). The following data indicate that guanine was decreased and xanthine was increased by guanase.


Purine bases in beer

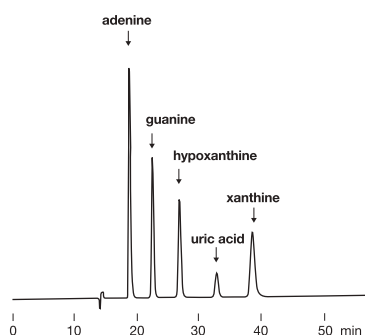

Normal beer

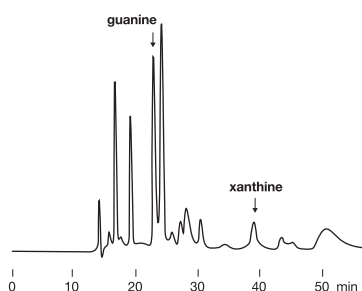

Guanase treated beer

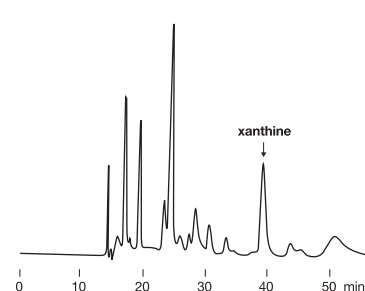


Column : Shodex Asahipak GS-320 HQ
Eluent : 150mM Sodium phosphate buffer (pH2.5)
Flow rate : 0.6mL/min
Detector : UV (260nm)
Column temp. : 35°C

Data provided by Kiyoko Kaneko Ph.D.,
 Faculty of Pharmaceutical Sciences, Teikyo University


Low molecular weight water-soluble dietary fiber

GS-220 HQ allows to elute monosaccharides, disaccharides, and sugar alcohols after the indigestible component fraction (indicated by an arrow on the chromatogram). This separation makes the method preferable for the quantification of low molecular weight water-soluble dietary fiber.

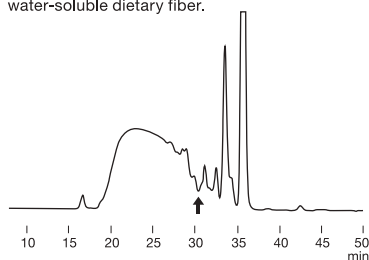

Column : Shodex Asahipak GS-220 HQ x 2
Eluent : H₂O
Flow rate : 0.5mL/min
Detector : RI
Column temp. : 60°C


"Umami"

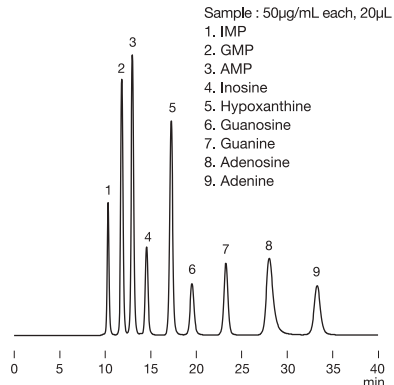

Column : Shodex Asahipak GS-320 HQ
Eluent : 10mM NaH₂PO₄ aq./10mM Na₂HPO₄ aq. =1000/31
Flow rate : 1.0mL/min
Detector : UV (260nm)
Column temp. : 40°C

Lignosulfonic acid

Sample : 100μL
 Lignosulfonic acid sodium salt 0.1%

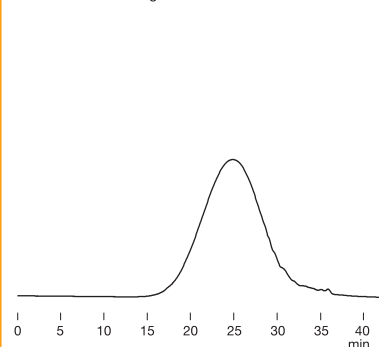

Column : Shodex Asahipak GS-520 HQ x 2
Eluent : 20mM Na₂HPO₄ aq.
Flow rate : 0.6mL/min
Detector : UV (254nm)
Column temp. : 40°C

● Aqueous/Organic SEC Columns

Features

- GF-HQ**
- Polymer-based SEC columns with high solvent durability
 - Works well with both aqueous and organic solvents

■ Standard columns

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7600000	Asahipak GF-210 HQ	≥ 19,000	5	180	7.5 × 300	H ₂ O
F7600001	Asahipak GF-310 HQ	≥ 19,000	5	400	7.5 × 300	H ₂ O/CH ₃ OH=70/30
F7600002	Asahipak GF-510 HQ	≥ 19,000	5	2,000	7.5 × 300	H ₂ O/CH ₃ OH=70/30
F7600003	Asahipak GF-710 HQ	≥ 11,000	9	10,000	7.5 × 300	H ₂ O/CH ₃ OH=70/30
F7600004	Asahipak GF-7M HQ	≥ 13,000	9	10,000	7.5 × 300	H ₂ O/CH ₃ OH=70/30
F6710018	Asahipak GF-1G 7B	(guard column)	9	—	7.5 × 50	H ₂ O/CH ₃ OH=70/30
F7600100	MSpak GF-310 4B	≥ 3,000	5	400	4.6 × 50	H ₂ O
F7600110	MSpak GF-310 4D	≥ 10,000	5	400	4.6 × 150	H ₂ O
F7600024	MSpak GF-310 4E	≥ 16,000	5	400	4.6 × 250	H ₂ O
F7600120	MSpak GF-310 2D	≥ 5,500	5	400	2.0 × 150	H ₂ O

GF-7M HQ is a mixed-gel column capable of analyzing samples over a wide range of molecular weight.

Base Material: Polyvinyl alcohol
Usable pH range: pH2-9

■ Semi-micro columns *The following semi-micro columns are made to order.

Product Code	Product Name	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F7600200	Asahipak GF-210 4D	5	180	4.6 × 150
F7600201	Asahipak GF-210 4E	5	180	4.6 × 250
F7760512	GF510A-4D	5	2,000	4.6 × 150
F7760511	GF510A-4E	5	2,000	4.6 × 250

Base Material: Polyvinyl alcohol

■ Preparative columns *Preparative columns are made to order.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6810030	Asahipak GS-310 20F	≥ 8,000	13	20.0 × 300	GF-310 HQ
F6810031	Asahipak GS-510 20F	≥ 8,000	13	20.0 × 300	GF-510 HQ
F6810032	Asahipak GS-710 20F	≥ 8,000	13	20.0 × 300	GF-710 HQ
F6810033	Asahipak GSM-700 20F	≥ 8,000	13	20.0 × 300	GF-7M HQ
F6810038	Asahipak GS-310 20G	≥ 14,000	13	20.0 × 500	GF-310 HQ
F6810039	Asahipak GS-510 20G	≥ 14,000	13	20.0 × 500	GF-510 HQ
F6810040	Asahipak GS-710 20G	≥ 14,000	13	20.0 × 500	GF-710 HQ
F6810041	Asahipak GSM-700 20G	≥ 14,000	13	20.0 × 500	GF-7M HQ
F6710020	Asahipak GS-10G 7B	(guard column)	20	7.5 × 50	(guard column)

Target molecular weight range and exclusion limit

● Measured with pullulan (eluent: ultrapure water)

Product Name	Target Molecular Weight Range	Exclusion Limit
GF-210	300 – 4,000	9,000
GF-310	300 – 30,000	40,000
GF-510	5,000 – 200,000	300,000
GF-710	100,000 – *(10,000,000)	*(10,000,000)
GF-7M	300 – *(10,000,000)	*(10,000,000)

*Please use the above table for reference purposes only when selecting columns.

*() Estimated value

● Measured with *PEG/PEO (eluent: DMF)

Product Name	Target Molecular Weight Range
GF-210	100 – 2,000
GF-310	200 – 4,000
GF-510	2,000 – 200,000
GF-710	20,000 – *(10,000,000)
GF-7M	200 – *(10,000,000)

*Please use the above table for reference purposes only when selecting columns.

*PEG: polyethylene glycol
*PEO: polyethylene oxide
*() Estimated value

Usable solvents

Solvent	GF-210	GF-310 GF-510 GF-710 GF-7M
Water (0 - 0.5M sodium concentration)	○	○
Methanol	○	○
Ethanol	○	○
Acetonitrile	○*	○
THF	○	○
DMF	○	○
Acetone	○	○
Chloroform	○*	○
Ethylacetate	○*	○
DMSO	○	0~50% ○

*When replacing acetonitrile, ethyl acetate or chloroform with water, replace with methanol first and then replace with water.


*When replacing water with ethyl acetate or chloroform, replace with methanol first and then replace with the required eluent condition.

(Note)

The usable solvents for preparative columns of GF-710 HQ, GS-710 20F and 20G, are water and methanol. Use of GSM-700 20F or 20G is recommended when other solvents are required.


Sodium polystyrene sulfonates

Polymers having both hydrophobic and hydrophilic functional groups may exhibit hydrophobic interactions with packing materials. When analyzing such polymers, addition of organic solvents to the eluent can suppress the hydrophobic interaction.

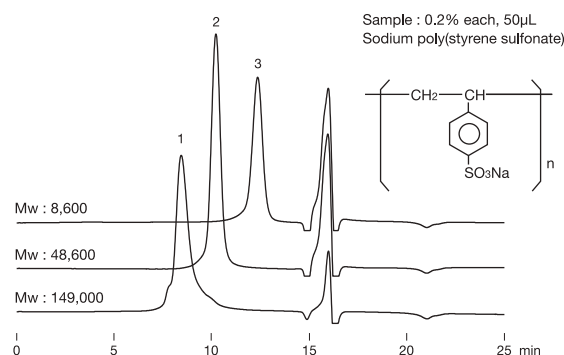


Column : Shodex Asahipak GF-510 HQ
Eluent : 50mM LiCl aq./CH₃CN=60/40
Flow rate : 0.6mL/min
Detector : UV (254nm)
Column temp. : 30°C

Calibration curves for GF-HQ series using pullulan (eluent: H₂O)

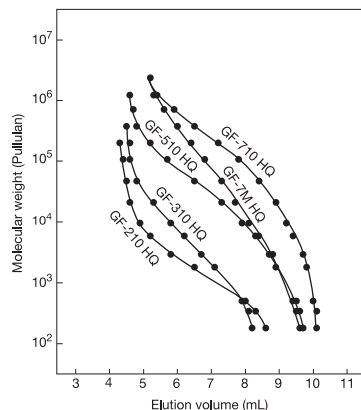


Column : Shodex Asahipak GF-HQ series
Eluent : H₂O
Flow rate : 0.6mL/min
Detector : RI
Column temp. : 30°C

Calibration curves for GF-HQ series using PEG/PEO (eluent: DMF)

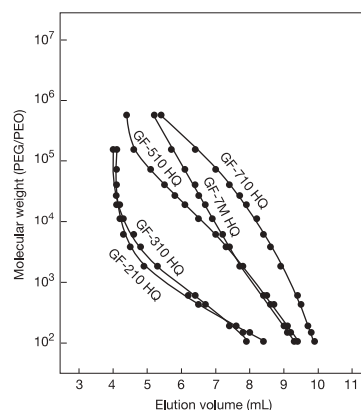

Column : Shodex Asahipak GF-HQ series
Eluent : DMF
Flow rate : 0.6mL/min
Detector : RI
Column temp. : 40°C


Polyacrylonitrile

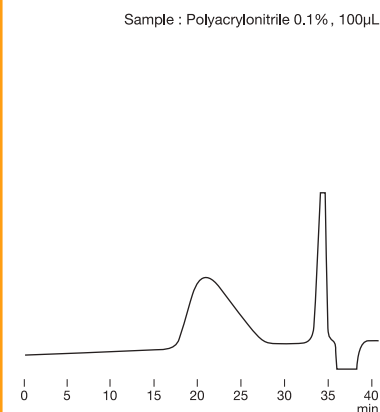

Column : Shodex Asahipak GF-710 HQ x 2
Eluent : 20mM LiBr in DMF
Flow rate : 0.6mL/min
Detector : RI
Column temp. : 40°C

Comparison of two GF column performances for the separation of maltoligosaccharides


GF-210 HQ demonstrates an improved separation of low molecular substances. The chromatograms below show that the peaks obtained by GF-210 HQ are separated with deeper notches compared to peaks obtained by GF-310 HQ. GF-210 HQ is capable of separating oligosaccharides (trisaccharides to hexasaccharides) while those oligosaccharides were eluted all together when analyzed by GF-310 HQ.

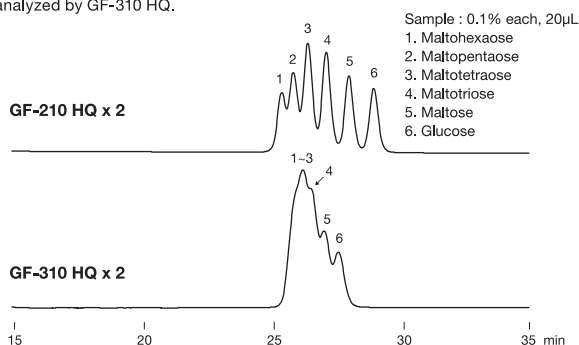

Column : Shodex Asahipak GF-210 HQ x 2
Shodex Asahipak GF-310 HQ x 2
Eluent : H₂O
Flow rate : 0.6mL/min
Detector : RI
Column temp. : 50°C

Comparison of polystyrene separation under three different solvent conditions

Sample : Polystyrene 1mg/mL each, 50μL
1. Mw : 1,090,000
2. Mw : 190,000
3. Mw : 37,900
4. Mw : 9,100
5. Mw : 2,980
6. Mw : 500

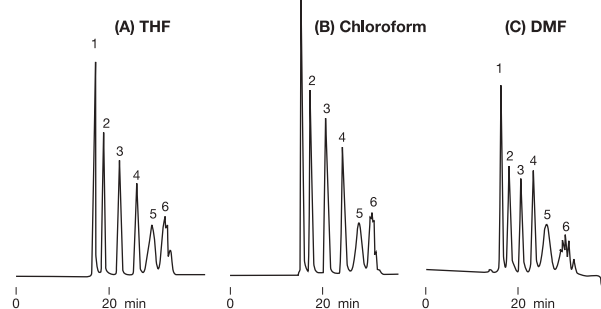

Column : Shodex Asahipak GF-510 HQ + GF-310 HQ
Eluent : (A); THF, (B); Chloroform, (C); DMF
Flow rate : 0.5mL/min
Detector : (A),(B) UV (254nm), (C) UV (270nm)
Column temp. : 30°C

Organic SEC (GPC) Columns (General Analysis): THF

Features

- KF-800**
 - Standard organic solvent SEC (GPC) column
 - Supports a wide range of applications from low to high molecular weight compounds
 - Fulfills USP L21 requirements

Standard columns

[KF-800 series: Shipping solvent Tetrahydrofuran (THF)]

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6028010	GPC KF-801	≥ 18,000	6	50	8.0 x 300
F6028020	GPC KF-802	≥ 18,000	6	150	8.0 x 300
F6028025	GPC KF-802.5	≥ 18,000	6	300	8.0 x 300
F6028030	GPC KF-803	≥ 18,000	6	500	8.0 x 300
F6027030	GPC KF-803L	≥ 18,000	6	500	8.0 x 300
F6028040	GPC KF-804	≥ 18,000	7	1,500	8.0 x 300
F6027040	GPC KF-804L	≥ 18,000	7	1,500	8.0 x 300
F6028050	GPC KF-805	≥ 11,000	10	5,000	8.0 x 300
F6027050	GPC KF-805L	≥ 11,000	10	5,000	8.0 x 300
F6028060	GPC KF-806	≥ 11,000	10	10,000	8.0 x 300
F6028090	GPC KF-806M	≥ 13,000	10	10,000	8.0 x 300
F6027060	GPC KF-806L	≥ 11,000	10	10,000	8.0 x 300
F6028070	GPC KF-807	≥ 6,000	18	20,000	8.0 x 300
F6027070	GPC KF-807L	≥ 6,000	18	20,000	8.0 x 300
F6700300	GPC KF-G 4A (GPC KF-G)	(guard column)	8	–	4.6 x 10
F6709350	GPC KF-800D	(solvent-peak separation column)	10	–	8.0 x 100

*The columns with 'L' or 'M' at the end of column names are mixed-gel column capable of analyzing samples over a wide range of molecular weight distribution.

*See page 54 for details of the solvent-peak separation columns.

*See pages 60 and 61 for details preparative columns.

*See page 68 for applicability of SEC (GPC) columns to solvent replacement.

Base Material: Styrene divinylbenzene copolymer

Target molecular weight range and exclusion limit


Measured with polystyrene (eluent: THF)

Product Name	Target Molecular Weight Range	Exclusion Limit	Product Name	Target Molecular Weight Range	Exclusion Limit
KF-801	100 – 700	1,500	KF-805	50,000 – 2,000,000	4,000,000
KF-802	300 – 3,000	5,000	KF-805L	300 – 2,000,000	4,000,000
KF-802.5	300 – 8,000	20,000	KF-806	150,000 – *(20,000,000)	*(20,000,000)
KF-803	1,000 – 50,000	70,000	KF-806M	1,000 – *(20,000,000)	*(20,000,000)
KF-803L	100 – 50,000	70,000	KF-806L	300 – *(20,000,000)	*(20,000,000)
KF-804	7,000 – 300,000	400,000	KF-807	300,000 – *(200,000,000)	*(200,000,000)
KF-804L	100 – 300,000	400,000	KF-807L	300 – *(200,000,000)	*(200,000,000)

*Please use the above tables for reference purposes only when selecting columns.


*() Estimated value

Calibration curves for KF-800 series using polystyrene

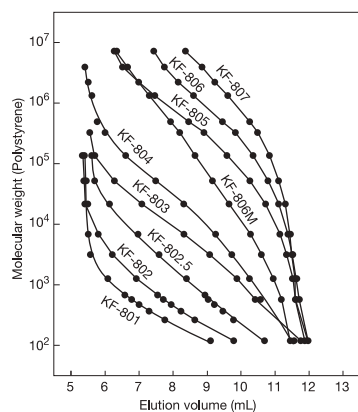


Column : Shodex GPC KF-800 series
Eluent : THF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Calibration curves for KF-800L (linear type) series using polystyrene

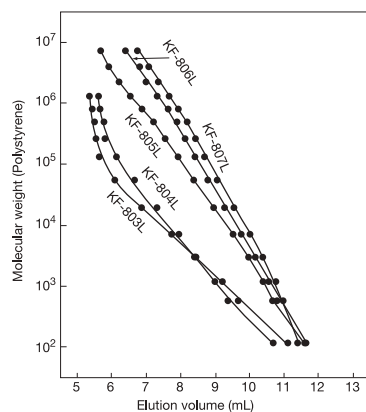


Column : Shodex GPC KF-800L series
Eluent : THF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Fat-soluble vitamins

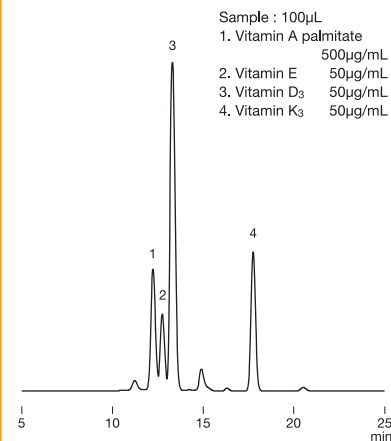


Column : Shodex GPC KF-801 x 2
Eluent : THF
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : 40°C

Polystyrene standards

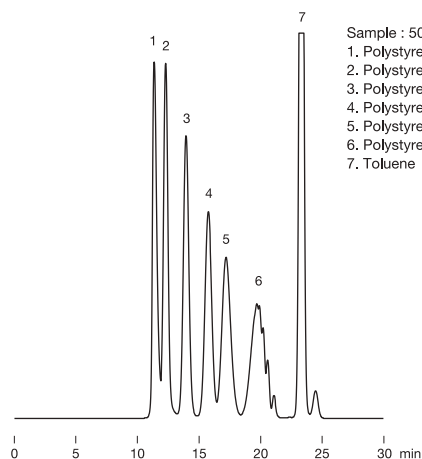


Column : Shodex GPC KF-803L x 2
Eluent : THF
Flow rate : 1.0mL/min
Detector : UV (254nm)
Column temp. : 40°C

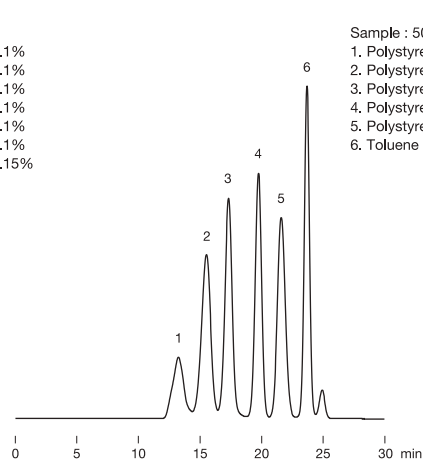


Column : Shodex GPC KF-807L x 2
Eluent : THF
Flow rate : 1.0mL/min
Detector : UV (254nm)
Column temp. : 40°C

Styrene isoprene ABA block copolymer

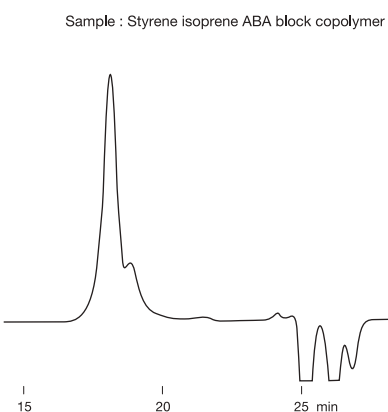


Column : Shodex GPC KF-806M x 2
Eluent : THF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 30°C

Polycarbonate resin

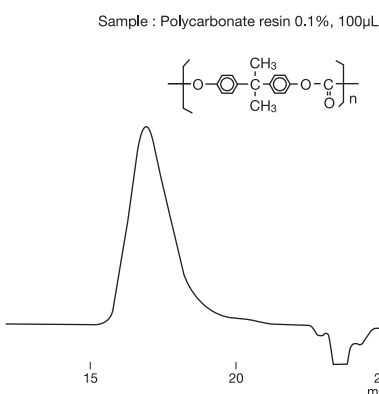

Column : Shodex GPC KF-806L x 2
Eluent : THF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Raw rubber

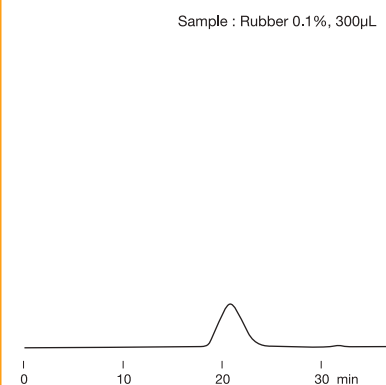

Column : Shodex GPC KF-806M x 2
 + KF-802
Eluent : Toluene
Flow rate : 1.0mL/min
Detector : RI
Column temp. : Room temp.

Organic SEC (GPC) Columns (General Analysis): Chloroform

Features

- K-800**
 - Standard organic solvent SEC (GPC) column
 - Supports a wide range of applications from low to high molecular weight compounds
 - Fulfills USP L21 requirements

Standard columns

[K-800 series: Shipping solvent Chloroform]

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6028110	GPC K-801	≥ 18,000	6	50	8.0 × 300
F6028120	GPC K-802	≥ 18,000	6	150	8.0 × 300
F6028125	GPC K-802.5	≥ 18,000	6	300	8.0 × 300
F6028130	GPC K-803	≥ 18,000	6	500	8.0 × 300
F6028194	GPC K-803L	≥ 18,000	6	500	8.0 × 300
F6028140	GPC K-804	≥ 18,000	7	1,500	8.0 × 300
F6028195	GPC K-804L	≥ 18,000	7	1,500	8.0 × 300
F6028150	GPC K-805	≥ 11,000	10	5,000	8.0 × 300
F6028196	GPC K-805L	≥ 11,000	10	5,000	8.0 × 300
F6028160	GPC K-806	≥ 11,000	10	10,000	8.0 × 300
F6028190	GPC K-806M	≥ 13,000	10	10,000	8.0 × 300
F6028197	GPC K-806L	≥ 11,000	10	10,000	8.0 × 300
F6028170	GPC K-807	≥ 6,000	18	20,000	8.0 × 300
F6028198	GPC K-807L	≥ 6,000	18	20,000	8.0 × 300
F6700401	GPC K-G 4A (GPC K-G)	(guard column)	8	–	4.6 × 10
F6709450	GPC K-800D	(solvent-peak separation column)	10	–	8.0 × 100

*The columns with 'L' or 'M' at the end of column names are mixed-gel column capable of analyzing samples over a wide range of molecular weight distribution.

*See page 54 for details of the solvent-peak separation columns.

*See pages 60 and 61 for details preparative columns.

*See page 68 for applicability of SEC (GPC) columns to solvent replacement.

Base Material: Styrene divinylbenzene copolymer

Target molecular weight range and exclusion limit

Measured with polystyrene (eluent: Chloroform)


Product Name	Target Molecular Weight Range	Exclusion Limit	Product Name	Target Molecular Weight Range	Exclusion Limit
K-801	100 – 700	1,500	K-805	50,000 – 2,000,000	4,000,000
K-802	300 – 3,000	5,000	K-805L	300 – 2,000,000	4,000,000
K-802.5	300 – 8,000	20,000	K-806	150,000 – *(20,000,000)	*(20,000,000)
K-803	1,000 – 50,000	70,000	K-806M	1,000 – *(20,000,000)	*(20,000,000)
K-803L	100 – 50,000	70,000	K-806L	300 – *(20,000,000)	*(20,000,000)
K-804	7,000 – 300,000	400,000	K-807	300,000 – *(200,000,000)	*(200,000,000)
K-804L	100 – 300,000	400,000	K-807L	300 – *(200,000,000)	*(200,000,000)

*Please use the above tables for reference purposes only when selecting columns.

*() Estimated value

Epoxy resin


Sample : Epikote 1001 0.1%, 100 μ L

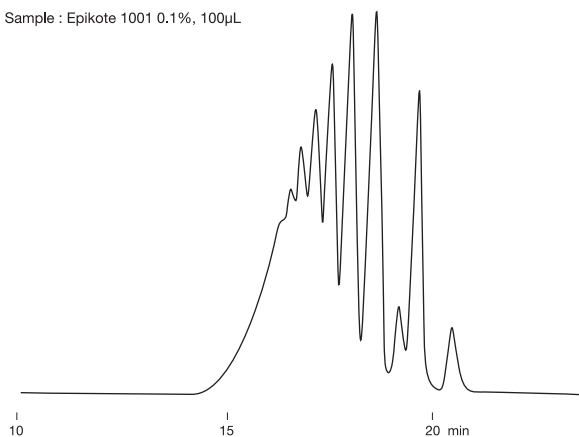

Column : Shodex GPC K-803L x 2
Eluent : Chloroform
Flow rate : 1.0mL/min
Detector : UV (254nm)
Column temp. : Room temp.

Low molecular polydimethylsiloxanes


Sample : 0.1% each, 100 μ L
1. Polydimethylsiloxane (MW:770)
2. Polydimethylsiloxane (MW:237)
3. Hexamethyldisiloxane (MW:162)

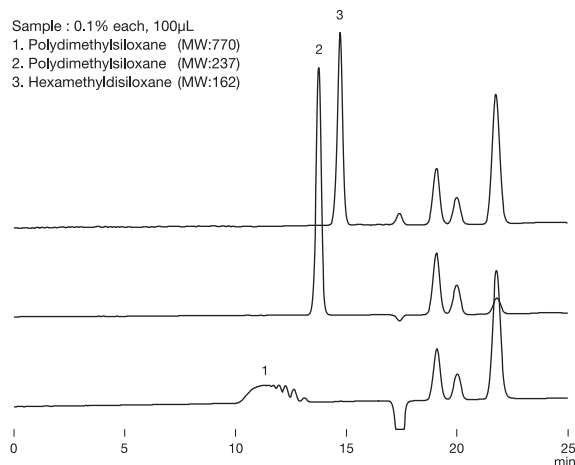

Column : Shodex GPC K-801 x 2
Eluent : Chloroform
Flow rate : 1.0mL/min
Detector : RI (polarity : -)
Column temp. : 40°C

Polylactic acid


Sample : Polylactic acid 0.2%, 50 μ L

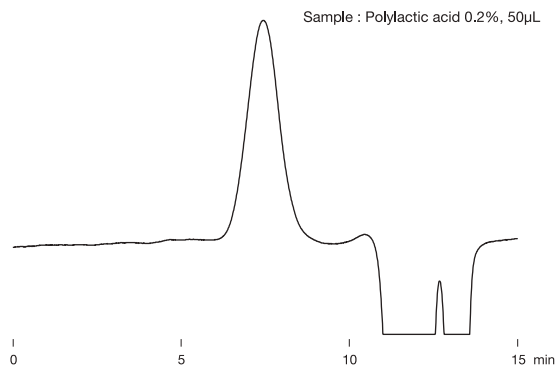

Column : Shodex GPC K-805L
Eluent : Chloroform
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 30°C

Silicone oil


Sample : Silicone oil 0.1%, 200 μ L

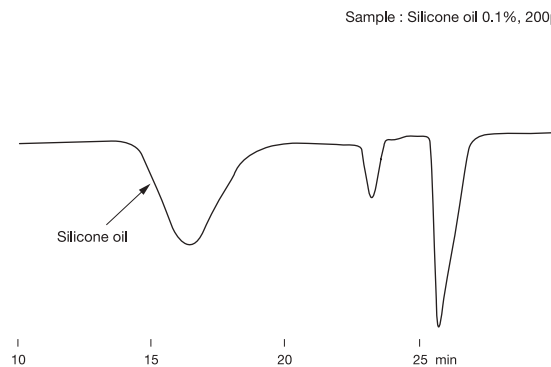

Column : Shodex GPC K-806M x 2
Eluent : Toluene
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 45°C

Recycling preparative chromatography of lauryl stearyl thiodipropionate

Sample : 5%, 500 μ L
1. Distearyl stearyl thiodipropionate
2. Lauryl stearyl thiodipropionate
3. Dilauryl thiodipropionate

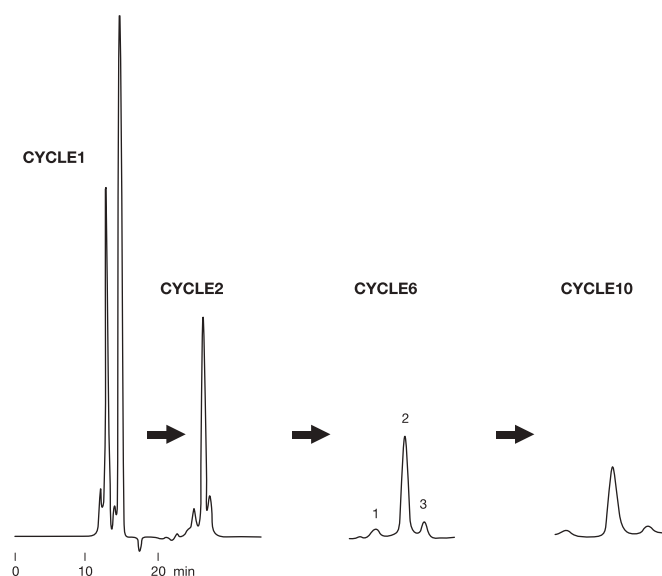

Column : Shodex GPC K-LG + K-2001
Eluent : Chloroform
Flow rate : 3.0mL/min
Detector : RI (preparative type)
Column temp. : 50°C

*See page 60 for K-2001

● Organic SEC (GPC) Columns (General Analysis): DMF

Features

- KD-800**
- Standard organic solvent SEC (GPC) column
 - Supports a wide range of applications from low to high molecular weight compounds
 - Fulfills USP L21 requirements

■ Standard columns

[KD-800 series: Shipping solvent Dimethylformamide (DMF)]

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6028210	GPC KD-801	≥ 17,000	6	50	8.0 x 300
F6028220	GPC KD-802	≥ 17,000	6	150	8.0 x 300
F6028225	GPC KD-802.5	≥ 17,000	6	300	8.0 x 300
F6028230	GPC KD-803	≥ 17,000	6	500	8.0 x 300
F6028240	GPC KD-804	≥ 17,000	7	1,500	8.0 x 300
F6028250	GPC KD-805	≥ 11,000	10	5,000	8.0 x 300
F6028260	GPC KD-806	≥ 11,000	10	10,000	8.0 x 300
F6028290	GPC KD-806M	≥ 13,000	10	10,000	8.0 x 300
F6028270	GPC KD-807	≥ 6,000	18	20,000	8.0 x 300
F6700411	GPC KD-G 4A (GPC KD-G)	(guard column)	8	–	4.6 x 10

*The column with 'M' at the end of column names is mixed-gel column capable of analyzing samples over a wide range of molecular weight distribution.

Base Material: Styrene divinylbenzene copolymer

*See page 68 for applicability of SEC (GPC) columns to solvent replacement.

Target molecular weight range and exclusion limit

● Measured with *PEG/PEO (eluent: DMF)

Product Name	Target Molecular Weight Range	Exclusion Limit	Product Name	Target Molecular Weight Range	Exclusion Limit
KD-801	100 – 1,500	2,500	KD-805	30,000 – *(4,000,000)	*(4,000,000)
KD-802	200 – 4,000	7,000	KD-806	30,000 – *(40,000,000)	*(40,000,000)
KD-802.5	400 – 10,000	20,000	KD-806M	1,000 – *(40,000,000)	*(40,000,000)
KD-803	1,000 – 50,000	70,000	KD-807	50,000 – *(200,000,000)	*(200,000,000)
KD-804	4,000 – 200,000	200,000			

*Please use the above tables for reference purposes only when selecting columns.

*PEG: polyethylene glycol
*PEO: polyethylene oxide
*() Estimated value

● Solvent-peak Separation Columns for Organic SEC (GPC)

Features


- KF-800D**
- Use this column in combination with a linear column
- K-800D**
- Accurate molecular weight distribution of polymers and oligomers are achieved by shifting the elutions of monomers, polymer additives, and solvent-peak in the lower molecular region

■ Solvent-peak separation columns

Product Code	Product Name	Column Combination	Particle Size (μm)	Column Size (mm) I.D. x Length	Shipping Solvent
F6709350	GPC KF-800D	KF-805L, 806L, 806M, 807L	10	8.0 x 100	THF
F6709450	GPC K-800D	K-805L, 806L, 806M, 807L	10	8.0 x 100	Chloroform

Base Material: Styrene divinylbenzene copolymer


Calibration curves for KD-800 series using PEG/PEO

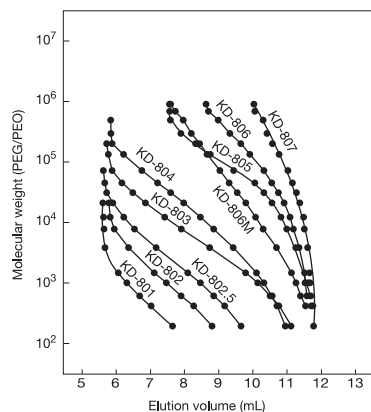

Column : Shodex GPC KD-800 series
Eluent : DMF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Polyvinylpyrrolidones


Sample : Polyvinylpyrrolidone 0.2% each
 (A) K-30 400μL
 (B) K-60 500μL
 (C) K-90 500μL

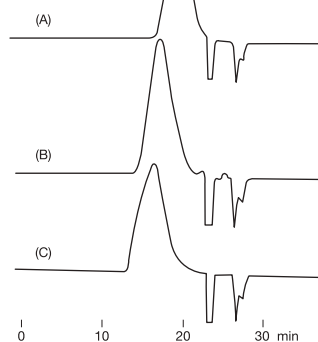

Column : Shodex GPC KD-806M x 2
Eluent : 10mM LiBr in DMF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 50°C


Melamine formaldehyde resin

Sample : 30μL
 Melamine-formaldehyde resin 1%

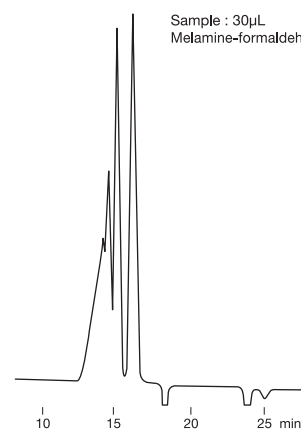

Column : Shodex GPC KD-802 x 2
Eluent : 10mM LiBr in DMF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 50°C

Celluloses

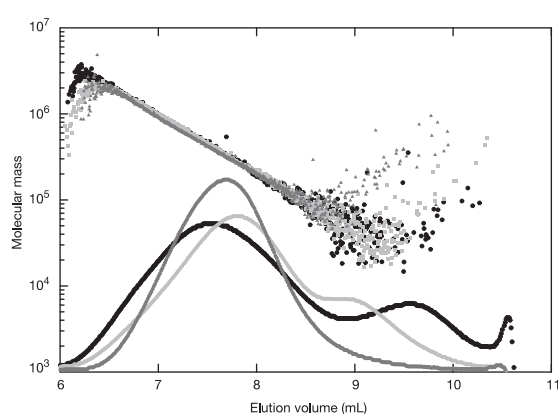

Sample : 100μL
 Cellulose ca. 0.05% each

Cellulose is difficult to dissolve and repeated solvent replacement is required to prepare the cellulose solution. The time required to completely dissolve cellulose depends on the solvent type, crystallinity and molecular weight of the cellulose. This can be 1 to 60 days.


Column : Shodex GPC KD-806M
Eluent : 1% LiCl in *DMI
Flow rate : 0.5mL/min
Detector : RI, MALS (Multi angle light scattering)
Column temp. : 60°C

*DMI 1,3-dimethyl-2-imidazolidinone

Data provided by Dr. Masahiko Yanagisawa,
 Isogai group,
 Graduate School of Agricultural and Life Sciences,
 The University of Tokyo

Phenoxy resin


Sample : 250μL
 Phenoxy resin 0.2%

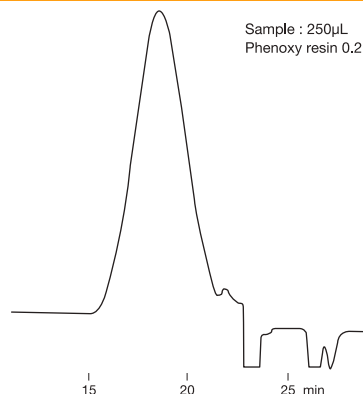

Column : Shodex GPC KD-806M x 2
Eluent : 10mM LiBr in DMF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 50°C

Potato starch



Sample : 100μL
 Potato starch in DMSO 0.1%
 *solved at 80°C

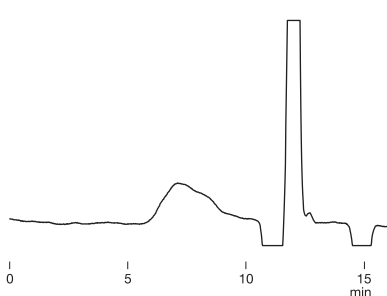

Column : Shodex GPC KD-806M
Eluent : 10mM LiBr in DMSO/DMF=75/25
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 50°C

Effects of solvent-peak separation column

Sample : Poly(vinyl chloride)

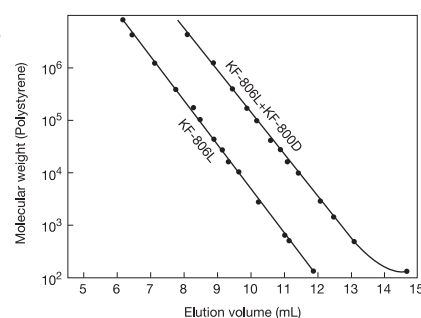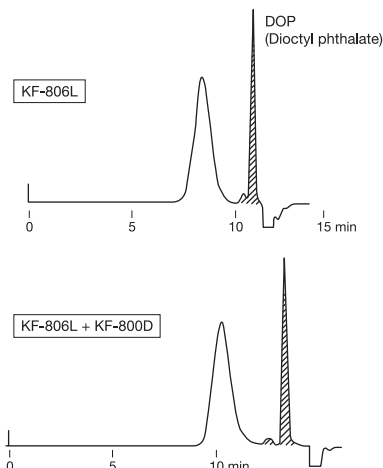

Column : Shodex GPC KF-806L
 Shodex GPC KF-806L + KF-800D
Eluent : THF
Flow rate : 1.0mL/min
Detector : RI

Organic SEC (GPC) Columns: Rapid Analysis, High Performance Analysis

Features

KF-600

- Achieves approximately halved analysis time compared with standard columns
- The amount of solvent used is reduced to about a third
- Improved applicability of solvent replacement
- Fulfills USP L21 requirements

KF-400HQ

- About 1.5 times better separation performance than standard columns, obtains higher resolution
- About 4 times better sensitivity than that of standard columns, supports high sensitivity analysis
- The amount of solvent used is reduced to about a third
- Improved applicability of solvent replacement
- Fulfills USP L21 requirements

Rapid analysis downsized columns

[KF-600 series]

© KF-600 series is recommended to be used with semi-micro type devices.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6028091	GPC KF-601	≥ 17,000	3	50	6.0 x 150
F6028092	GPC KF-602	≥ 17,000	3	150	6.0 x 150
F6028093	GPC KF-602.5	≥ 17,000	3	300	6.0 x 150
F6028094	GPC KF-603	≥ 17,000	3	500	6.0 x 150
F6028095	GPC KF-604	≥ 16,000	3	1,500	6.0 x 150
F6028096	GPC KF-605	≥ 7,000	10	5,000	6.0 x 150
F6028097	GPC KF-606	≥ 7,000	10	10,000	6.0 x 150
F6028098	GPC KF-606M	≥ 8,000	10	10,000	6.0 x 150
F6028099	GPC KF-607	≥ 5,000	18	20,000	6.0 x 150
F6700300	GPC KF-G 4A (GPC KF-G)	(guard column)	8	–	4.6 x 10

High performance semi-micro columns

[KF-400HQ series]

© KF-400HQ series is recommended to be used with semi-micro type devices.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6028111	GPC KF-401HQ	≥ 25,000	3	50	4.6 x 250
F6028112	GPC KF-402HQ	≥ 25,000	3	150	4.6 x 250
F6028114	GPC KF-402.5HQ	≥ 25,000	3	300	4.6 x 250
F6028116	GPC KF-403HQ	≥ 25,000	3	500	4.6 x 250
F6028118	GPC KF-404HQ	≥ 25,000	3	1,500	4.6 x 250
F6028119	GPC KF-405LHQ	≥ 10,000	10	5,000	4.6 x 250
F6028122	GPC KF-406LHQ	≥ 10,000	10	10,000	4.6 x 250
F6700300	GPC KF-G 4A (GPC KF-G)	(guard column)	8	–	4.6 x 10

[KF-600 series and KF-400HQ series]

*The columns with 'L' or 'M' at the end of column names are mixed-gel column capable of analyzing samples over a wide range of molecular weight distribution.

*See page 68 for applicability of SEC (GPC) columns to solvent replacement.

[KF-600 series and KF-400HQ series]

Base Material: Styrene divinylbenzene copolymer
Shipping Solvent: Tetrahydrofuran (THF)

Target molecular weight range and exclusion limit

Measured with polystyrene (eluent: THF)


Product Name	Target Molecular Weight Range	Exclusion Limit
KF-601	100 – 700	1,500
KF-602	200 – 1,500	4,000
KF-602.5	300 – 10,000	20,000
KF-603	600 – 50,000	70,000
KF-604	7,000 – 500,000	1,000,000
KF-605	50,000 – 2,000,000	4,000,000
KF-606	150,000 – *(20,000,000)	*(20,000,000)
KF-606M	1,000 – *(20,000,000)	*(20,000,000)
KF-607	300,000 – *(200,000,000)	*(200,000,000)

Product Name	Target Molecular Weight Range	Exclusion Limit
KF-401HQ	100 – 700	1,500
KF-402HQ	200 – 1,500	4,000
KF-402.5HQ	300 – 10,000	20,000
KF-403HQ	600 – 50,000	70,000
KF-404HQ	7,000 – 500,000	1,000,000
KF-405LHQ	300 – 2,000,000	4,000,000
KF-406LHQ	300 – *(20,000,000)	*(20,000,000)

*Please use the above tables for reference purposes only when selecting columns.


*() Estimated value

Calibration curves for KF-600 series using polystyrene

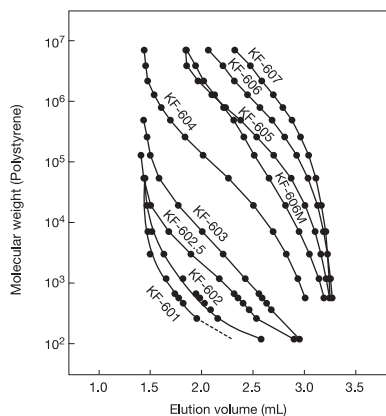

Column : Shodex GPC KF-600 series
 Eluent : THF
 Flow rate : 0.5mL/min
 Detector : RI (small cell volume)
 Column temp. : 40°C

Calibration curves for KF-400HQ series using polystyrene

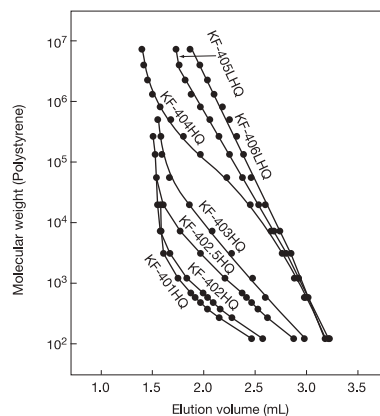


Column : Shodex GPC KF-400HQ series
 Eluent : THF
 Flow rate : 0.3mL/min
 Detector : RI (small cell volume)
 Column temp. : 40°C

Comparison of standard, rapid analysis, and high performance type columns

Standard type
 KF-802.5 x 2
 50μL injection

High performance type
 KF-402.5HQ x 2
 10μL injection

Rapid analysis type
 KF-602.5 x 2
 10μL injection

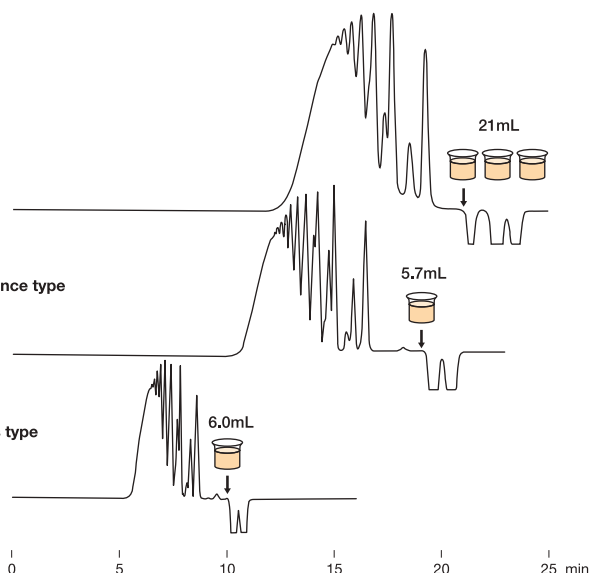


Sample : EPON1001 0.2%

KF-602.5 provides rapid analysis by reducing the analysis time; less than half of the analysis time of KF-802.5. Having 1.5 times more theoretical plate number than standard column, KF-402.5HQ provides improved resolution especially for the separation of small to medium molecular weight substances. Rapid analysis and high performance type columns use less than one third of solvent per analysis compared to standard type columns do.

Column : Shodex GPC KF-802.5 x 2
 Shodex GPC KF-402.5HQ x 2
 Shodex GPC KF-602.5 x 2
 Eluent : THF
 Flow rate : 1.0mL/min (KF-802.5)
 0.3mL/min (KF-402.5HQ)
 0.6mL/min (KF-602.5)
 Detector : RI (conventional type) (KF-802.5)
 RI (small cell volume) (KF-402.5HQ, KF-602.5)
 Column temp. : 40°C

Styrene acrylonitrile copolymer


Sample : Styrene-Acrylonitrile (30:70) copolymer

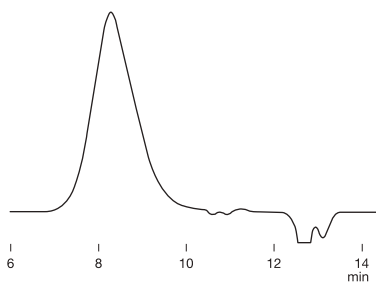

Column : Shodex GPC KF-606M x 2
 Eluent : 10mM LiBr in DMF
 Flow rate : 0.5mL/min
 Detector : RI (small cell volume)
 Column temp. : 40°C

Liquid paraffin

Sample : Liquid paraffin 1%, 5μL

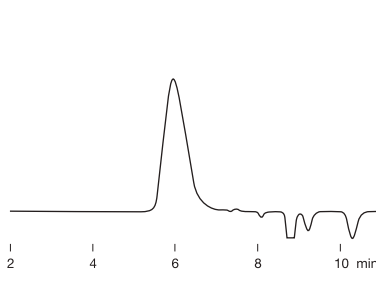


Column : Shodex GPC KF-401HQ
 Eluent : Chloroform
 Flow rate : 0.3mL/min
 Detector : RI (small cell volume)
 Column temp. : 40°C

Phthalates

Sample : 10μL

1. Dioctyl phthalate 0.1%
2. Dibutyl phthalate 0.1%
3. Dipropyl phthalate 0.1%
4. Diethyl phthalate 0.1%
5. Dimethyl phthalate 0.1%
6. Propylbenzene 0.2%
7. Ethylbenzene 0.2%
8. Toluene 0.2%
9. Benzene 0.2%

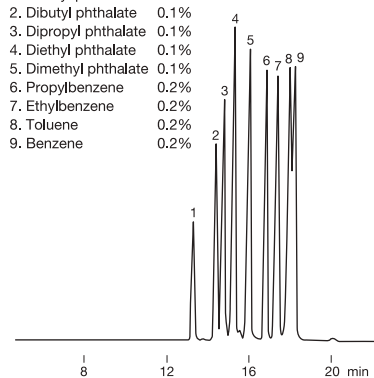

Column : Shodex GPC KF-401HQ x 2
 Eluent : THF
 Flow rate : 0.3mL/min
 Detector : UV (254nm) (small cell volume)
 Column temp. : 40°C

Organic SEC (GPC) Columns: Ultra-Rapid Analysis

Features

New HK-400

- Newly developed styrene divinylbenzene copolymer monodisperse particles
- Analysis time reduced to about one sixth of conventional column's analysis time
- Low column pressure even under high flow rate does not require its use with UHPLC device
- The amount of solvent used is reduced to about a sixth
- HK-HFIP404L is filled with HFIP
- Fulfills USP L21 requirements

Ultra-Rapid analysis semi-micro columns

[Shipping Solvent: Tetrahydrofuran (THF)]

© HK-400 series is recommended to be used with semi-micro type devices.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6025010	New GPC HK-401	≥ 9,000	3	50	4.6 x 150
F6026040	New GPC HK-404L	≥ 9,000	3.5	2,000	4.6 x 150
F6025050	New GPC HK-405	≥ 7,000	3	5,000	4.6 x 150

*The column with 'L' at the end of column names is mixed-gel column capable of analyzing samples over a wide range of molecular weight distribution.

Base Material: Styrene divinylbenzene copolymer

[Shipping Solvent: hexafluoroisopropanol (HFIP)]

© HK-HFIP404L is recommended to be used with semi-micro type devices.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6026140	New GPC HK-HFIP404L	≥ 9,000	3.5	800	4.6 x 150

*The column with 'L' at the end of column names is mixed-gel column capable of analyzing samples over a wide range of molecular weight distribution.


Base Material: Styrene divinylbenzene copolymer

*See page 66 for details of other columns filled with HFIP.

Guard filter for HK series

Product Code	Product Name	Contents
F6700200	New GPC HK-G	One holder and one filter
F6700100	New GPC HK-G filter	3 filters

Removes insoluble components in the sample

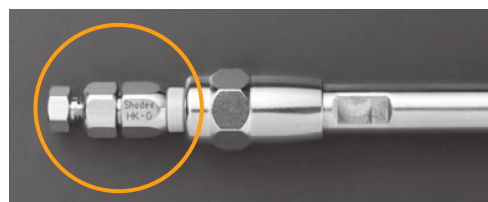

*Allows direct attachment to the analytical column

Target molecular weight range and exclusion limit

Measured with polystyrene (eluent: THF)

Product Name	Target Molecular Weight Range	Exclusion Limit
HK-401	100 – 1,500	2,000
HK-404L	100 – 1,000,000	1,000,000
HK-405	10,000 – 2,500,000	4,000,000

*Please use the above table for reference purposes only when selecting columns.


Measured with *PMMA (eluent: HFIP)

Product Name	Target Molecular Weight Range	Exclusion Limit
HK-HFIP404L	5,000 – 200,000	200,000

*Please use the above table for reference purposes only when selecting columns.


*PMMA: Polymethylmethacrylate

Calibration curves for HK-400 series using polystyrene (eluent: THF)

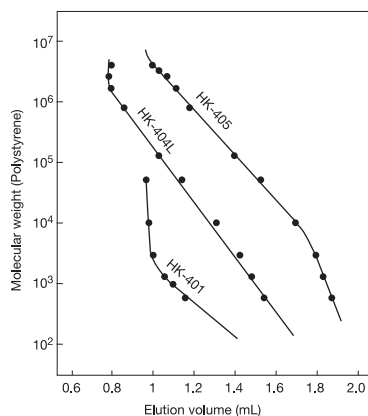


Column : Shodex GPC HK-400 series
Eluent : THF
Flow rate : 1.0mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Calibration curves for HK-400 series using PEG/PEO (eluent: DMF)

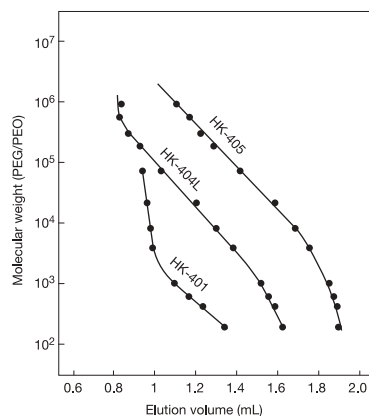


Column : Shodex GPC HK-400 series
Eluent : DMF
Flow rate : 1.0mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Calibration curve for HK-HFIP404L using PMMA (eluent: HFIP)

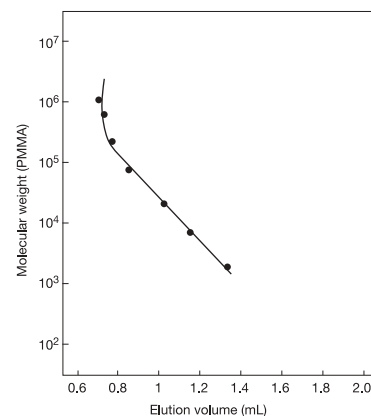


Column : Shodex GPC HK-HFIP404L
Eluent : 5mM CF₃COONa in HFIP
Flow rate : 0.3mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Comparison of HK-404L and conventional column (KF-805L)

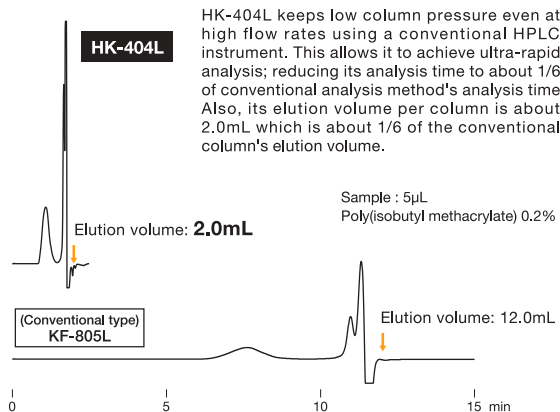


Column : Shodex GPC HK-404L, KF-805L
Eluent : THF
Flow rate : 1.0mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Poly(butyl methacrylate)

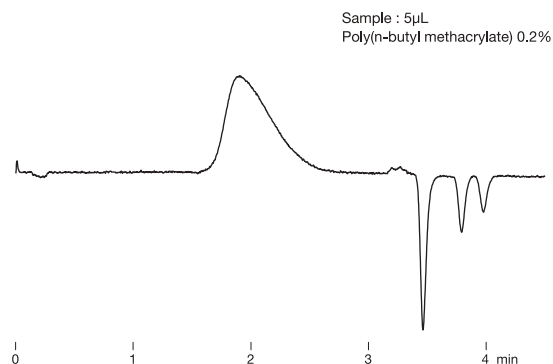


Column : Shodex GPC HK-404L x 2
Eluent : THF
Flow rate : 1.0mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Styrene butyl methacrylate copolymer

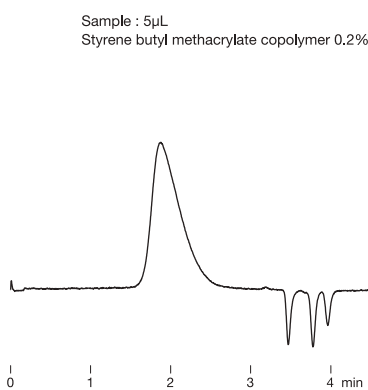


Column : Shodex GPC HK-404L x 2
Eluent : THF
Flow rate : 1.0mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Polyamide (Nylon 6/9)

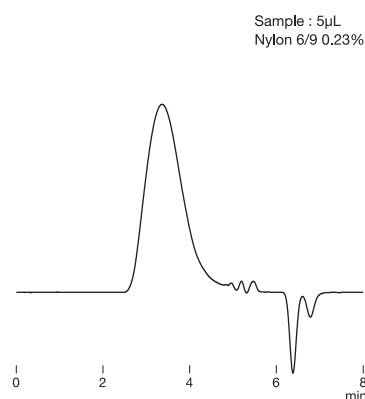

Column : Shodex GPC HK-HFIP404L
Eluent : 5mM CF₃COONa in HFIP
Flow rate : 0.3mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Polyamide (Nylon 11)

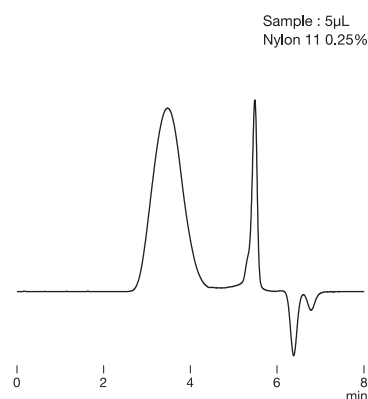

Column : Shodex GPC HK-HFIP404L
Eluent : 5mM CF₃COONa in HFIP
Flow rate : 0.3mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Organic SEC (GPC) Columns: Preparative Columns

■ Preparative columns *Preparative columns are made to order.

[KF-2000 series: Shipping solvent Tetrahydrofuran (THF)]

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6102401	GPC KF-2001	≥ 18,000	6	20.0 x 300	KF-801
F6102402	GPC KF-2002	≥ 18,000	6	20.0 x 300	KF-802
F6102425	GPC KF-2002.5	≥ 18,000	6	20.0 x 300	KF-802.5
F6102403	GPC KF-2003	≥ 18,000	6	20.0 x 300	KF-803
F6102404	GPC KF-2004	≥ 14,000	7	20.0 x 300	KF-804
F6102405	GPC KF-2005	≥ 10,000	10	20.0 x 300	KF-805
F6102406	GPC KF-2006	≥ 10,000	10	20.0 x 300	KF-806
F6102409	GPC KF-2006M	≥ 10,000	10	20.0 x 300	KF-806M
F6700406	GPC KF-G 8B (GPC KF-LG)	(guard column)	15	8.0 x 50	(guard column)

*See page 50 for details of GPC KF-800 series.

Base Material: Styrene divinylbenzene copolymer

[K-2000 series: Shipping solvent Chloroform]

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6102301	GPC K-2001	≥ 18,000	6	20.0 x 300	K-801
F6102312	GPC K-2002	≥ 18,000	6	20.0 x 300	K-802
F6102315	GPC K-2002.5	≥ 18,000	6	20.0 x 300	K-802.5
F6102303	GPC K-2003	≥ 18,000	6	20.0 x 300	K-803
F6102304	GPC K-2004	≥ 14,000	7	20.0 x 300	K-804
F6102305	GPC K-2005	≥ 10,000	10	20.0 x 300	K-805
F6102306	GPC K-2006	≥ 10,000	10	20.0 x 300	K-806
F6102309	GPC K-2006M	≥ 10,000	10	20.0 x 300	K-806M
F6700407	GPC K-G 8B (GPC K-LG)	(guard column)	15	8.0 x 50	(guard column)

*See page 52 for details of GPC K-800 series.

Base Material: Styrene divinylbenzene copolymer

■ Preparative columns *Preparative columns are made to order.

[H-2000 series: Shipping solvent Chloroform]

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6102001	GPC H-2001	≥ 13,000	15	20.0 × 500	K-801
F6102002	GPC H-2002	≥ 13,000	15	20.0 × 500	K-802
F6102025	GPC H-2002.5	≥ 13,000	15	20.0 × 500	K-802.5
F6102003	GPC H-2003	≥ 13,000	15	20.0 × 500	K-803
F6102004	GPC H-2004	≥ 13,000	15	20.0 × 500	K-804
F6102005	GPC H-2005	≥ 13,000	15	20.0 × 500	K-805
F6102006	GPC H-2006	≥ 13,000	15	20.0 × 500	K-806
F6102009	GPC H-2006M	≥ 12,000	15	20.0 × 500	K-806M
F6700310	GPC H-G 8B (GPC H-G)	(guard column)	15	8.0 × 50	(guard column)

*See page 52 for details of GPC K-800 series.

Base Material: Styrene divinylbenzene copolymer

[KF-5000 series: Shipping solvent Tetrahydrofuran (THF)]

[Customized columns]

Product Code	Product Name	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6108010	GPC KF-5001	15	50.0 × 300	KF-801
F6108020	GPC KF-5002	15	50.0 × 300	KF-802
F6108025	GPC KF-5002.5	15	50.0 × 300	KF-802.5
F6108030	GPC KF-5003	15	50.0 × 300	KF-803
F6108040	GPC KF-5004	15	50.0 × 300	KF-804
F6700408	GPC KF-G 20C (GPC KF-LLG)	15	20.0 × 100	(guard column)

*See page 50 for details of GPC KF-800 series.

Base Material: Styrene divinylbenzene copolymer

[K-5000 series: Shipping solvent Chloroform]

[Customized columns]

Product Code	Product Name	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard Column
F6109010	GPC K-5001	15	50.0 × 300	K-801
F6109020	GPC K-5002	15	50.0 × 300	K-802
F6109025	GPC K-5002.5	15	50.0 × 300	K-802.5
F6109030	GPC K-5003	15	50.0 × 300	K-803
F6109040	GPC K-5004	15	50.0 × 300	K-804
F6700409	GPC K-G 20C (GPC K-LLG)	15	20.0 × 100	(guard column)

*See page 52 for details of GPC K-800 series.

Base Material: Styrene divinylbenzene copolymer

Organic SEC (GPC) Columns: Linear Calibration Type

Features

- LF**
- Packed with unique multi-pore gels with a wide pore-size distribution
 - Highly linear calibration curve without inflection points
 - Achieves highly precise molecular weight distribution determination
 - Enables analysis over a broad range of molecular weights
 - Rapid analysis column (LF-604) and high performance analysis column (LF-404) are also available
 - LF-604 and LF-404 enables reduction of solvent use
 - Fulfills USP L21 requirements

Standard columns

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6021041	GPC LF-804	≥ 17,000	6	3,000	8.0 × 300
F6709621	GPC LF-G	(guard column)	6	–	4.6 × 10

*See page 68 for applicability of SEC (GPC) columns to solvent replacement.

Base Material: Styrene divinylbenzene copolymer
Shipping Solvent: Tetrahydrofuran (THF)

Rapid analysis downsized column

◎ LF-604 is recommended to be used with semi-micro type devices.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6021042	GPC LF-604	≥ 9,000	6	3,000	6.0 × 150
F6709621	GPC LF-G	(guard column)	6	–	4.6 × 10

*See page 68 for applicability of SEC (GPC) columns to solvent replacement.

Base Material: Styrene divinylbenzene copolymer
Shipping Solvent: Tetrahydrofuran (THF)

High performance semi-micro column

◎ LF-404 is recommended to be used with semi-micro type devices.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6021043	GPC LF-404	≥ 14,000	6	3,000	4.6 × 250
F6709621	GPC LF-G	(guard column)	6	–	4.6 × 10

*See page 68 for applicability of SEC (GPC) columns to solvent replacement.

Base Material: Styrene divinylbenzene copolymer
Shipping Solvent: Tetrahydrofuran (THF)

Target molecular weight range and exclusion limit


Measured with polystyrene (eluent: THF)

Product Name	Target Molecular Weight Range	Exclusion Limit
LF-804	300 – 2,000,000	2,000,000
LF-604	300 – 2,000,000	2,000,000
LF-404	300 – 2,000,000	2,000,000

*Please use the above table for reference purposes only when selecting columns.


Schematic diagram of linear calibration type packing

Connecting linear calibration type columns (LF series)

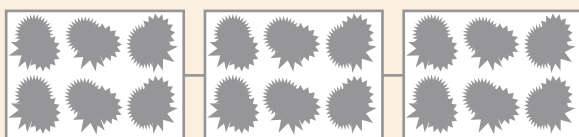

The linear calibration type column covers a broad range of molecular weights with only one kind of packing material.


Connecting mixed-gel columns (KF-804L, etc.)



Connecting different single pore-size columns (KF-804 + KF-803 + KF-802, etc.)




Calibration curve for LF-804 using polystyrene

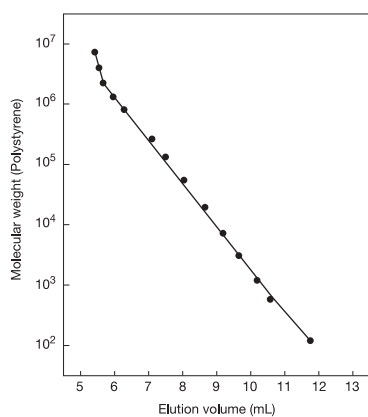


Column : Shodex GPC LF-804
Eluent : THF
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Calibration curves for LF-604 and LF-404 using polystyrene

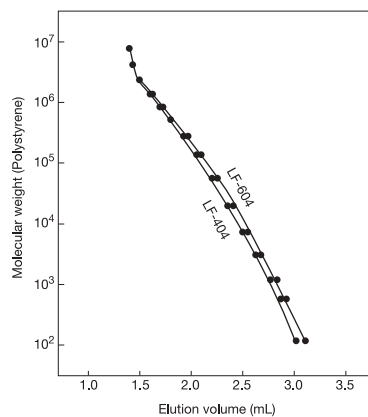


Column : Shodex GPC LF-604, LF-404
Eluent : THF
Flow rate : 0.5mL/min (LF-604)
0.3mL/min (LF-404)
Detector : RI (small cell volume)
Column temp. : 40°C

Polyurethane

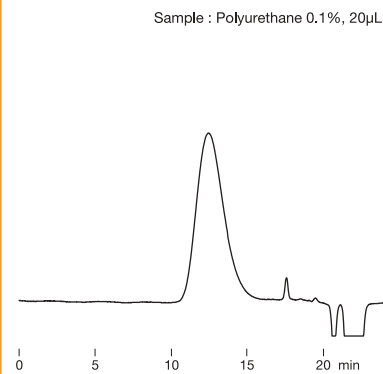


Column : Shodex GPC LF-404 x 2
Eluent : THF
Flow rate : 0.3mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Xylan

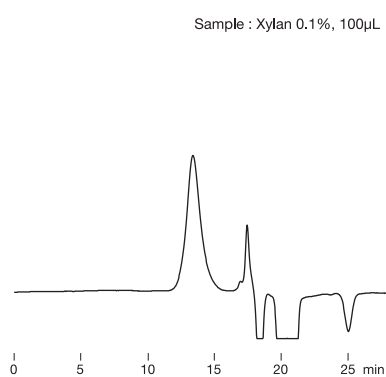


Column : Shodex GPC LF-804
Eluent : 20mM H₃PO₄ + 20mM LiBr
in DMSO/DMF=80/20
Flow rate : 0.6mL/min
Detector : RI
Column temp. : 50°C

Polyamide (Nylon6/6)

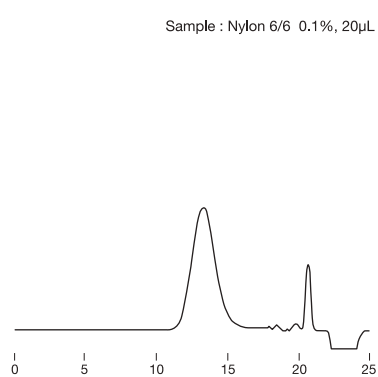


Column : Shodex GPC LF-404
Eluent : 5mM CF₃COONa in HFIP
Flow rate : 0.15mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Polymethyl methacrylate

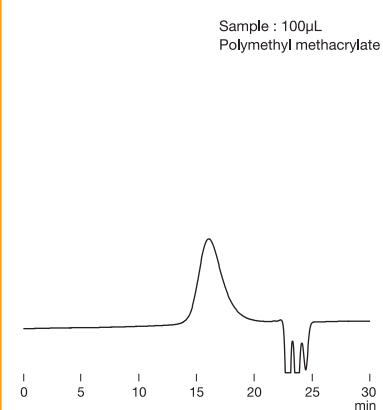


Column : Shodex GPC LF-804 x 2
Eluent : Methyl ethyl ketone
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Polyamic acid

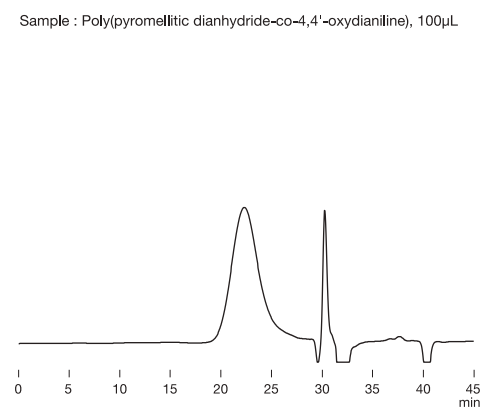

Column : Shodex GPC LF-804 x 2
Eluent : 30mM LiBr + 30mM H₃PO₄ in NMP
Flow rate : 0.7mL/min
Detector : RI
Column temp. : 50°C

Effects of using multiple LF-404 columns for the separation of polystyrenes

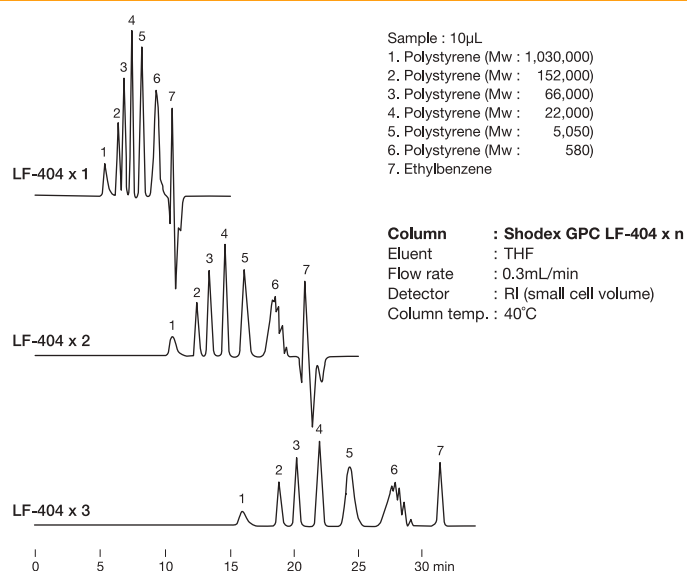

Organic SEC (GPC) Columns: High Temperature/Ultra High Temperature Analysis

Features

- HT-800**
 - Wide product lineup to support a broad range of molecular weight analysis
 - Fulfills USP L21 requirements
- UT-800**
 - Dedicated to SEC analysis at high/ultra high temperatures with a maximum usable temperature of 210°C
 - Suitable for the analysis of ultra high molecular weight polymer containing samples
 - Fulfills USP L21 requirements

Standard columns

Product Code	Product Name	Plate Number (TP/column)	Usable Temperature (°C)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6208700	GPC HT-803	≥ 7,000	100 ~ 150	13	500	8.0 x 300
F6208710	GPC HT-804	≥ 7,000	100 ~ 150	13	1,500	8.0 x 300
F6208720	GPC HT-805	≥ 7,000	100 ~ 150	13	5,000	8.0 x 300
F6208730	GPC HT-806	≥ 7,000	100 ~ 150	13	10,000	8.0 x 300
F6208740	GPC HT-806M	≥ 7,000	100 ~ 150	13	10,000	8.0 x 300
F6208770	GPC HT-807	≥ 4,000	100 ~ 150	18	20,000	8.0 x 300
F6709410	GPC HT-G	(guard column)	100 ~ 150	13	–	8.0 x 50
F6208600	GPC UT-802.5	≥ 4,400	100 ~ 210	30	300	8.0 x 300
F6208610	GPC UT-806M	≥ 4,400	100 ~ 210	30	10,000	8.0 x 300
F6208620	GPC UT-807	≥ 3,300	100 ~ 210	30	20,000	8.0 x 300
F6709400	GPC UT-G	(guard column)	100 ~ 210	30	–	8.0 x 50
F6208390	GPC AT-806MS	≥ 6,000	*Ta ~ 150	12	10,000	8.0 x 250
F6700280	GPC AT-G	(guard column)	*Ta ~ 150	15	–	8.0 x 50

*The columns with 'M' at the end of column names is mixed-gel column capable of analyzing samples over a wide range of molecular weight distribution.

Base Material: Styrene divinylbenzene copolymer
Shipping Solvent: Toluene
*Ta: Ambient temperature

Target molecular weight range and exclusion limit


Measured with polystyrene (eluent: o-Dichlorobenzene (ODCB))

Product Name	Target Molecular Weight Range	Exclusion Limit
HT-803	1,000 – 50,000	70,000
HT-804	7,000 – 300,000	400,000
HT-805	50,000 – 2,000,000	4,000,000
HT-806	150,000 – *(20,000,000)	*(20,000,000)
HT-806M	1,000 – *(20,000,000)	*(20,000,000)
HT-807	300,000 – *(200,000,000)	*(200,000,000)
UT-802.5	300 – 10,000	20,000
UT-806M	1,000 – *(20,000,000)	*(20,000,000)
UT-807	500,000 – *(200,000,000)	*(200,000,000)
AT-806MS	1,000 – *(20,000,000)	*(20,000,000)

*Please use the above table for reference purposes only when selecting columns.


*() Estimated value

Calibration curves for HT-800 series using polystyrene

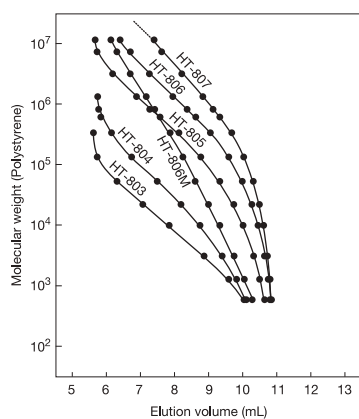


Column : Shodex GPC HT-800 series
Eluent : 0.1% BHT in ODCB
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 140°C

Calibration curves for UT-800 series using polystyrene

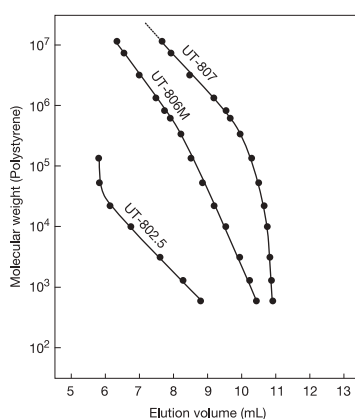

Column : Shodex GPC UT-800 series
Eluent : 0.1% BHT in ODCB
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 140°C

Calibration curve for AT-806MS using polystyrene



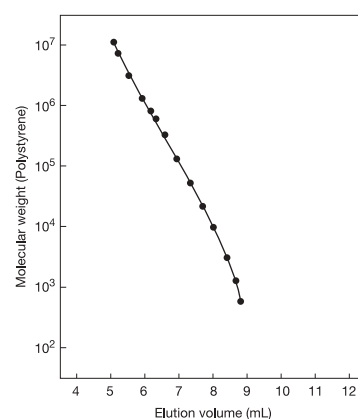


Column : Shodex GPC AT-806MS
Eluent : 0.1% BHT in ODCB
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 140°C

Effects of gel particle size in high temperature GPC columns

High temperature GPC columns are suitable for the analysis of high molecular weight polymers that are difficult to be dissolved in ambient temperature solvents; examples of such polymers are polyethylene and polypropylene. The GPC UT-800 series packed with large particle size (30μm) are recommended for the analysis of macromolecules. The large particle size prevents potential molecular shear degradation of the sample.


Sample :
1. Polystyrene (MW : 20,000,000)
2. High density polyethylene (HDPE-A)

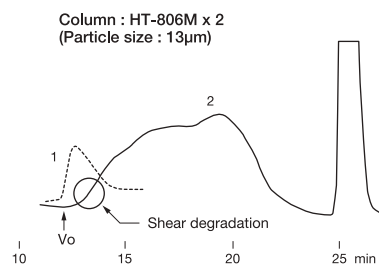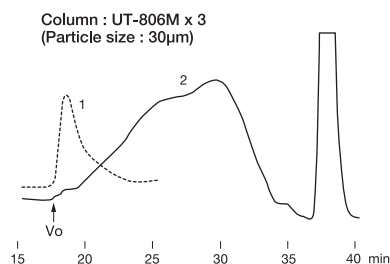

Column : Shodex GPC UT-806M
Shodex GPC HT-806M
Shodex GPC AT-806MS
Eluent : 0.1% BHT in ODCB
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 140°C

High density polyethylene


Sample : High density polyethylene (HDPE-B)

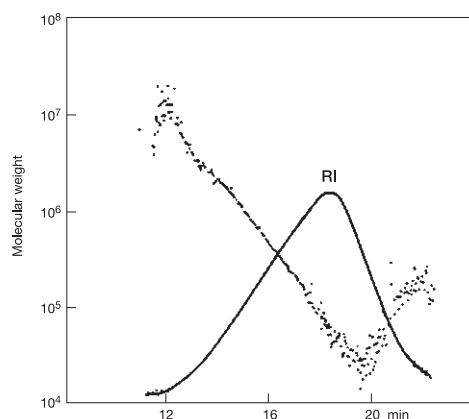

Column : Shodex GPC UT-806M x 2
Eluent : 0.1% BHT in ODCB
Flow rate : 1.0mL/min
Detector : RI, MALS (Multi angle light scattering)
Column temp. : 145°C

Low density polyethylene

Sample : Low density polyethylene (LDPE-C)

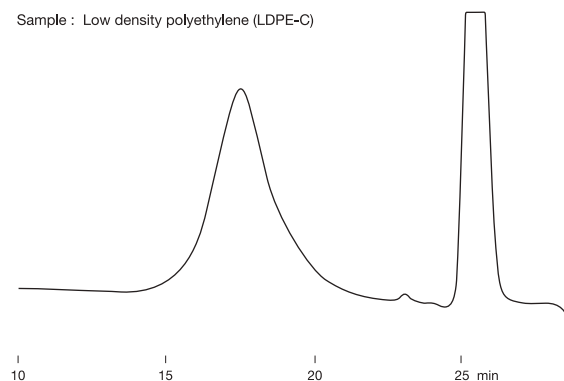

Column : Shodex GPC HT-806M x 2
Eluent : 0.1% BHT in ODCB
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 140°C

Organic SEC (GPC) Columns: HFIP

Features

- HFIP-800**
- Columns exclusively used with hexafluoroisopropanol (HFIP)
 - Fulfills USP L21 requirements

- HFIP-600**
- Rapid analysis, solvent saving type
 - Fulfills USP L21 requirements

Standard columns

[HFIP-800 series]

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6028530	GPC HFIP-803	≥ 12,000	10	500	8.0 x 300
F6028540	GPC HFIP-804	≥ 12,000	7	1,500	8.0 x 300
F6028550	GPC HFIP-805	≥ 10,000	10	5,000	8.0 x 300
F6028560	GPC HFIP-806	≥ 10,000	10	10,000	8.0 x 300
F6028590	GPC HFIP-806M	≥ 10,000	10	10,000	8.0 x 300
F6028570	GPC HFIP-807	≥ 4,000	18	20,000	8.0 x 300
F6700500	GPC HFIP-G 8B (GPC HFIP-LG)	(guard column)	15	–	8.0 x 50

*The columns with 'M' at the end of column names is mixed-gel column capable of analyzing samples over a wide range of molecular weight distribution.

Base Material: Styrene divinylbenzene copolymer
Shipping Solvent: Hexafluoroisopropanol (HFIP)

Rapid analysis downsized columns

[HFIP-600 series]

© HFIP-600 series is recommended to be used with semi-micro type devices.

Product Code	Product Name	Plate Number (TP/column)	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length
F6021030	GPC HFIP-603	≥ 12,000	3	500	6.0 x 150
F6021040	GPC HFIP-604	≥ 12,000	3	1,500	6.0 x 150
F6021050	GPC HFIP-605	≥ 5,000	10	5,000	6.0 x 150
F6021060	GPC HFIP-606	≥ 5,000	10	10,000	6.0 x 150
F6021080	GPC HFIP-606M	≥ 6,000	10	10,000	6.0 x 150
F6021070	GPC HFIP-607	≥ 3,000	18	20,000	6.0 x 150
F6700511	GPC HFIP-G 4A (GPC HFIP-G)	(guard column)	8	–	4.6 x 10

*The columns with 'M' at the end of column names is mixed-gel column capable of analyzing samples over a wide range of molecular weight distribution.

*See page 58 for details of a column enclosed with HFIP.

Base Material: Styrene divinylbenzene copolymer
Shipping Solvent: Hexafluoroisopropanol (HFIP)

Target molecular weight range and exclusion limit

Measured with *PMMA (eluent: HFIP)


Product Name	Target Molecular Weight Range	Exclusion Limit
HFIP-803	1,000 – 30,000	60,000
HFIP-804	20,000 – 200,000	300,000
HFIP-805	20,000 – 600,000	1,000,000
HFIP-806	70,000 – *(8,000,000)	*(8,000,000)
HFIP-806M	1,000 – *(8,000,000)	*(8,000,000)
HFIP-807	70,000 – *(50,000,000)	*(50,000,000)

Product Name	Target Molecular Weight Range	Exclusion Limit
HFIP-603	1,000 – 30,000	60,000
HFIP-604	20,000 – 200,000	300,000
HFIP-605	20,000 – 600,000	1,000,000
HFIP-606	70,000 – *(8,000,000)	*(8,000,000)
HFIP-606M	1,000 – *(8,000,000)	*(8,000,000)
HFIP-607	70,000 – *(50,000,000)	*(50,000,000)

*Please use the above tables for reference purposes only when selecting columns.


*PMMA: Polymethylmethacrylate
*() Estimated value

Calibration curves for HFIP-800 series using PMMA

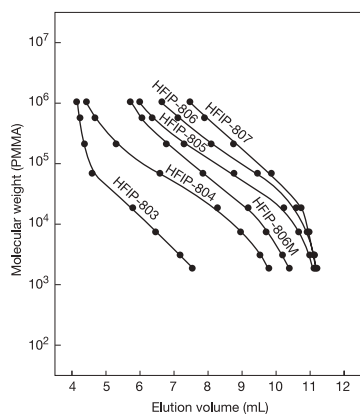

Column : Shodex GPC HFIP-800 series
Eluent : HFIP
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C


Calibration curves for HFIP-600 series using PMMA

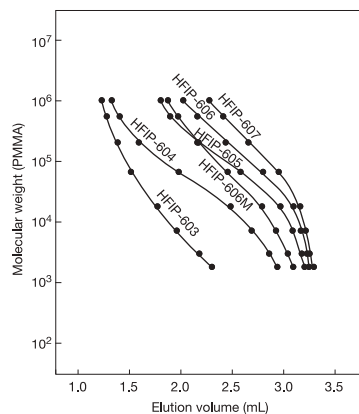

Column : Shodex GPC HFIP-600 series
Eluent : HFIP
Flow rate : 0.3mL/min (HFIP-603, 604)
 0.5mL/min (HFIP-605, 606, 606M, 607)
Detector : RI (small cell volume)
Column temp. : 40°C

Polyethylene terephthalate (PET)


Sample : Polyethylene terephthalate 0.2%, 20μL

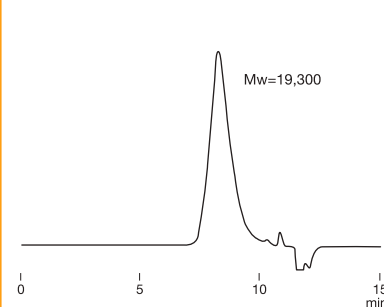

Column : Shodex GPC HFIP-606M x 2
Eluent : 5mM CF₃COONa in HFIP
Flow rate : 0.6mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Polyamide (effects of added salt)

Sample : Polycaprolactum (Nylon 6)

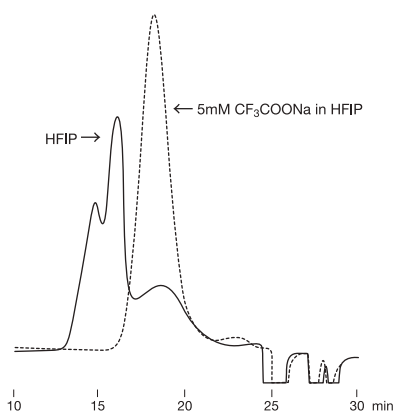


Some samples analyzed under SEC mode with HFIP solvent may show abnormal peaks resulting from the ionic interaction. This interaction can be suppressed by adding sodium trifluoroacetate to the HFIP eluent.

Column : Shodex GPC HFIP-806M x 2
Eluent : HFIP (solid line), 5mM CF₃COONa in HFIP (broken line)
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Polybutylene terephthalate (PBT)


Sample : Polybutylene terephthalate 0.05%, 500μL

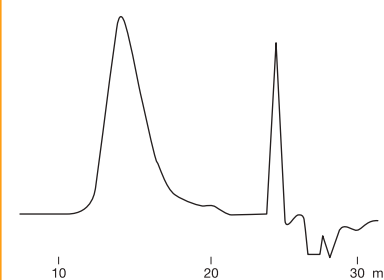


Column : Shodex GPC HFIP-805 + HFIP-803
Eluent : 5mM CF₃COONa in HFIP
Flow rate : 1.0mL/min
Detector : RI
Column temp. : 40°C

Polyamides (Nylon 6/10 and Nylon 6)

Sample : Nylon 6/10 0.2%, 20μL

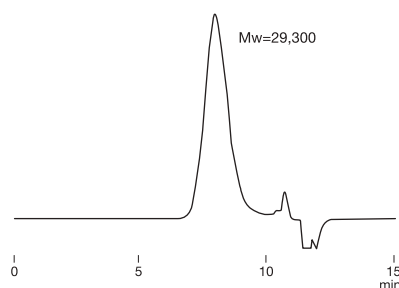


Sample : Nylon 6 0.2%, 20μL

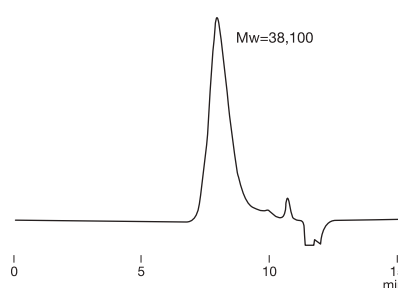

Column : Shodex GPC HFIP-606M x 2
Eluent : 5mM CF₃COONa in HFIP
Flow rate : 0.6mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Polyacetal

Sample : Polyacetal 0.2%, 20μL

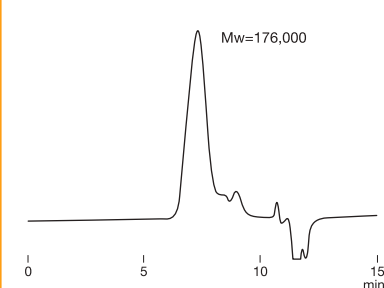

Column : Shodex GPC HFIP-606M x 2
Eluent : 5mM CF₃COONa in HFIP
Flow rate : 0.6mL/min
Detector : RI (small cell volume)
Column temp. : 40°C

Solvent Replacement Applicability of SEC (GPC) Columns

Solvent	Product Name									
	Shipping Solvent: THF							Shipping Solvent: DMF		
	KF-801	KF-802 KF-802.5 KF-803L KF-804L	KF-803	KF-804 KF-805 KF-806 KF-807 KF-806M KF-805L KF-806L KF-807L	KF-601 KF-602 KF-602.5	KF-603 KF-604 KF-605 KF-606 KF-607 KF-606M	LF-804 LF-604 LF-404	KD-801 KD-802 KD-802.5	KD-803	KD-804 KD-805 KD-806 KD-807 KD-806M
	Shipping Solvent: Chloroform				Shipping Solvent: THF					
	K-801	K-802 K-802.5 K-803L K-804L	K-803	K-804 K-805 K-806 K-807 K-806M K-805L K-806L K-807L	KF-401HQ KF-402HQ KF-402.5HQ	KF-403HQ KF-404HQ KF-405LHQ KF-406LHQ				
Tetrahydrofuran (THF)	○	○	○	○	○	○	○	×	×	○
Chloroform	○	○	○	○	○	○	○	×	×	○
Carbon tetrachloride	×	○	○	○			○	×	×	○
Benzene	○	○	○	○	○	○		×	○	○
Toluene	○	○	○	○	○	○	○	×	○	○
p-Xylene	×	○	○	○	○	○		×	○	○
o-Dichlorobenzene (ODCB)	×	×	○	○	○	○		×	○	○
Trichlorobenzene (TCB)	×	×	○	○	○	○		×	○	○
Dioxane	×	○	○	○				×	○	○
Diethyl ether	×	×	○	○				×	○	○
Ethyl acetate	×	×	○	○				×	×	○
Acetone	×	×	○	○	○	○		×	○	○
Methyl ethyl ketone	×	×	○	○	○	○	○	×	○	○
Dimethylformamide (DMF)	×	×	○	○	○ *	○ *	○ *	○	○	○
Dimethylacetamide (DMAc)	×	×	○	○	○ *	○ *	○ *	×	○	○
Hexafluoroisopropanol (HFIP)	×	×	×	○	×	△ *	○ *	×	○	○
m-Cresol	×	×	○	○				×	○	○
o-Chlorophenol	×	×	○	○				×	○	○
Quinolin	×	×	○	○				×	○	○
N-Methylpyrrolidone (NMP)	×	×	○	○	○ *	○ *	○ *	×	○	○
Dimethylsulfoxide (DMSO)	×	×	×	△	△ *	○ *	○ *	×	○	○
30% m-Cresol/Chloroform	×	○	○	○			○	×	○	○
30% o-Chlorophenol/Chloroform	×	○	○	○			○	×	○	○
30% HFIP/Chloroform	×	○	○	○				×	○	○
Hexane	×	×	×	×	×	×	×	×	×	×
Acetonitrile	×	×	×	×	×	×	×	×	×	×
Methanol	×	×	×	×	×	×	×	×	×	×
Water	×	×	×	×	×	×	×	×	×	×

○: Solvent replacement possible

△: Solvent replacement possible, but this may cause column performance to deteriorate slightly

*: Usable at 40°C or higher

×: Solvent replacement not possible

Calibration Standards for SEC

[Polystyrene (PS)]


Features

- For organic solvent SEC (GPC)
- Less branched polystyrene with anionic polymerization
- Easily soluble in tetrahydrofuran (THF), chloroform, toluene, and o-dichlorobenzene (ODCB)

Standard kit

Product Code	Product Name	Contents	MW Range
F8601105	STANDARD SL-105	0.5g x 10 kinds	580 – 19,900
F8602105	STANDARD SM-105	0.5g x 10 kinds	1,150 – 2,380,000
F8603075	STANDARD SH-75	0.5g x 7 kinds	508,000 – 6,870,000

Structural formula of S series



SL-105

Std. No.	Mp	Mw/Mn
S-20	19,900	1.03
S-13	13,000	1.02
S-9.6	9,590	1.02
S-7.6	7,640	1.02
S-4.7	4,730	1.03
S-3.0	2,970	1.04
S-1.9	1,920	1.04
S-1.4	1,440	1.05
S-0.9	860	1.07
S-0.6	580	1.11

SM-105

Std. No.	Mp	Mw/Mn
S-2380	2,380,000	1.08
S-1390	1,390,000	1.05
S-730	730,000	1.05
S-270	270,000	1.02
S-139	139,000	1.03
S-45	45,100	1.02
S-20	19,500	1.02
S-6.3	6,320	1.03
S-3.0	2,970	1.04
S-1.2	1,150	1.08

SH-75

Std. No.	Mp	Mw/Mn
S-6870	6,870,000	1.09
S-5190	5,190,000	1.03
S-3750	3,750,000	1.05
S-2350	2,350,000	1.04
S-2000	2,000,000	1.03
S-991	991,000	1.05
S-508	508,000	1.05

(Note)
Molecular weights (Mp, Mw/Mn) of each standard kit may vary depending on production lots.

[Polymethylmethacrylate (PMMA)]

Features

- For organic solvent SEC (GPC)
- Narrow molecular weight distribution range
- Easily soluble in hexafluoroisopropanol (HFIP) and dimethylformamide (DMF)

Standard kit

Product Code	Product Name	Contents	MW Range
F8604075	STANDARD M-75	0.5g x 7 kinds	2,880 – 1,020,000

(Note)
Molecular weights (Mp, Mw/Mn) of a standard kit may vary depending on production lots.

Std. No.	Mp	Mw/Mn
M-1020	1,020,000	1.04
M-505	505,000	1.02
M-224	224,000	1.02
M-67	66,700	1.03
M-18	17,800	1.04
M-6.1	6,140	1.11
M-2.9	2,880	1.08

[Pullulan]

Features

- For aqueous SEC (GFC)
- Unbranched pullulan standard
- High solubility in water eliminates the possibility of recrystallization


Standard kit

Product Code	Product Name	Contents	MW Range
F8400000	STANDARD P-82	0.2g x 8 kinds	6,100 – 642,000

Single type

Product Code	Product Name	Contents	Mp	Mw/Mn
F8400800	STD P-800	0.5g	642,000	1.23
F8400400	STD P-400	0.5g	337,000	1.12
F8400200	STD P-200	0.5g	194,000	1.09
F8400100	STD P-100	0.5g	107,000	1.13
F8400050	STD P-50	0.5g	47,100	1.07
F8400020	STD P-20	0.5g	22,000	1.08
F8400010	STD P-10	0.5g	9,600	1.09
F8400005	STD P-5	0.5g	6,100	1.05

Structural formula of P series



Std. No.	Mp	Mw/Mn
STD P-800	642,000	1.23
STD P-400	337,000	1.12
STD P-200	194,000	1.09
STD P-100	107,000	1.13
STD P-50	47,100	1.07
STD P-20	22,000	1.08
STD P-10	9,600	1.09
STD P-5	6,100	1.05

(Note)
Molecular weights (Mp, Mw/Mn) of a standard kit or each single type may vary depending on production lots.

● Anion Exchange Chromatography Columns

Features

QA-825 DEAE-825	- Suitable for analyzing relatively high molecular weight compounds: proteins, peptides, DNA, and RNA - Usable in a wide pH range from pH 2 to 12 - QA-825 fulfills USP L23 requirements
DEAE3N-4T	- Non-porous base material - For rapid analysis
DEAE-2B	- Non-porous base material - Can be used with UHPLC (available under hyperbaric conditions up to 30 MPa)
ES-502N 7C	- Compared to IEC series columns, polyvinyl alcohol is used as base material and this offers different separation pattern - Low hydrophobic interaction of proteins allows analysis under mild conditions
WA-624	Suitable for anion exchange analysis of low molecular weight compounds such as nucleotides

■ Standard columns

[Strong anion exchange resin] Functional Group: Quaternary ammonium

Product Code	Product Name	Ion Exchange Capacity (meq/g)	Base Material	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6110011	IEC QA-825	0.45	Polyhydroxymethacrylate	12	5,000	8.0 × 75	50mM Na ₂ SO ₄ aq.

[Weak anion exchange resin] Functional Group: Diethylaminoethyl

Product Code	Product Name	Ion Exchange Capacity (meq/g)	Base Material	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6118255	IEC DEAE-825	0.6	Polyhydroxymethacrylate	8	5,000	8.0 × 75	50mM Na ₂ SO ₄ aq.
F6112100	IEC DEAE3N-4T	0.4	Polyhydroxymethacrylate	2.5	–	4.6 × 35	H ₂ O
F7640002	Asahipak ES-502N 7C	0.55	Polyvinyl alcohol	9	2,000	7.5 × 100	50mM 1,3-Diaminopropane + 50mM NaCl (pH10.0)
F6356240	AXpak WA-624	1.2	Polyhydroxymethacrylate	10	2,000	6.0 × 150	0.1M Sodium phosphate buffer (pH3.0)/CH ₃ CN =80/20
F6700245	AXpak WA-G (guard column)	–	Polyhydroxymethacrylate	10	–	4.6 × 10	0.1M Sodium phosphate buffer (pH3.0)/CH ₃ CN =80/20

[Weak anion exchange resin] Functional Group: Diethylaminoethyl (UHPLC column)


Product Code	Product Name	Ion Exchange Capacity (meq/g)	Base Material	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6112110	PIKESS DEAE-2B	0.4	Polyhydroxymethacrylate	2.5	–	2.0 × 50	H ₂ O

■ Preparative columns *Preparative columns are made to order.

Product Code	Product Name	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard column
F6548000	IEC QA-2025	20	20.0 × 150	QA-825
F6709602	IEC QA-G 8B (IEC QA-LG)	20	8.0 × 50	(guard column)
F6548001	IEC DEAE-2025	20	20.0 × 150	DEAE-825
F6709603	IEC DEAE-G 8B (IEC DEAE-LG)	20	8.0 × 50	(guard column)
F6840004	Asahipak ES-502N 20C	13	20.0 × 100	ES-502N 7C
F6710021	Asahipak GS-20G 7B	20	7.5 × 50	(guard column)


Proteins in human serum

Sample : Human serum 0.5%, 200 μ L
 1. IgG
 2. Transferrin
 3. (Unknown)
 4. Serum albumin

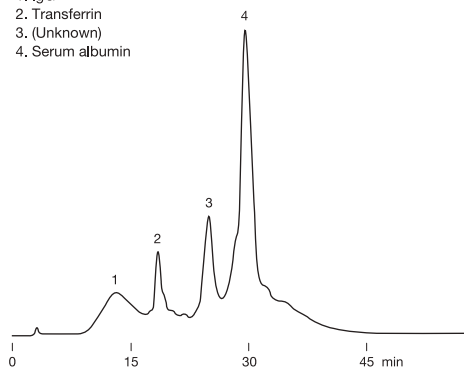

Column : Shodex IEC QA-825
Eluent : (A); 20mM Tris-HCl buffer (pH8.6)
 (B); (A) + 0.5M NaCl
 Linear gradient; 100% (A) to 50% (B), 60min
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : Room temp.

Effects of eluent pH on DEAE-825 analysis

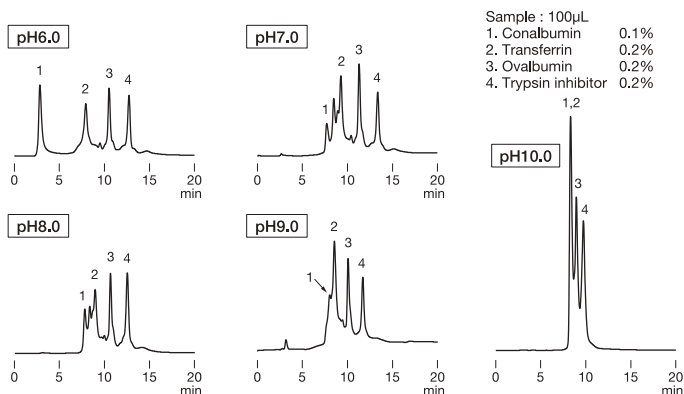


Sample : 100 μ L
 1. Conalbumin 0.1%
 2. Transferrin 0.2%
 3. Ovalbumin 0.2%
 4. Trypsin inhibitor 0.2%

Column : Shodex IEC DEAE-825
Eluent : (A); 20mM Piperazine-HCl buffer (pH6.0), 20mM Bis-Tris-HCl buffer (pH7.0)
 20mM Tris-HCl buffer (pH8.0), 20mM Ethanolamine-HCl buffer (pH9.0)
 20mM 1,3-Diaminopropane-HCl buffer (pH10.0)
 (B); (A) + 0.5M NaCl
 Linear gradient; (A) to (B), 20min
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : 25°C

Comparison of porous DEAE-825 and non-porous DEAE3N-4T for protein separation


IEC DEAE3N-4T is a weak anion exchange column, having diethylaminoethyl functional group modified on non-porous gel. The non-porous gel enables rapid analysis of proteins and peptides. DEAE3N-4T is also suitable for the analysis of small-volume samples, as it provides sharp peaks even with small injection volume.

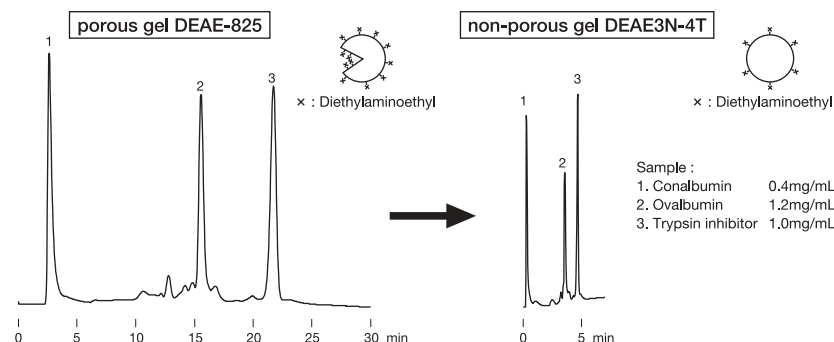

Column : Shodex IEC DEAE-825
Eluent : (A); 20mM Piperazine-HCl buffer (pH6.0)
 (B); (A) + 0.5M NaCl
 Linear gradient; (A) to (B), 60min
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : Room temp.
Injection vol. : 100 μ L

Column : Shodex IEC DEAE3N-4T
Eluent : (A); 25mM Piperazine-HCl buffer (pH6.0)
 (B); (A) + 0.5M NaCl
 Linear gradient; (A) to (B), 10min
Flow rate : 1.5mL/min
Detector : UV (280nm)
Column temp. : Room temp.
Injection vol. : 20 μ L

Gibberellin Isomers

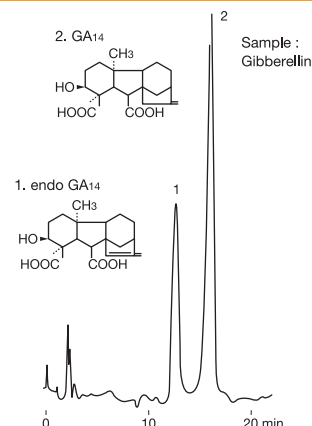


Sample : Gibberellin

Column : Shodex Asahipak ES-502N 7C
Eluent : CH₃COOH/H₂O/CH₃OH
 =0.1/0.4/99.5
Flow rate : 1.5mL/min
Detector : UV (210nm)
Column temp. : 50°C

Data was provided by Prof. Yamaguchi,
 Faculty of Agriculture, University of Tokyo.


Mercaptoalbumin and non-mercaptoalbumin

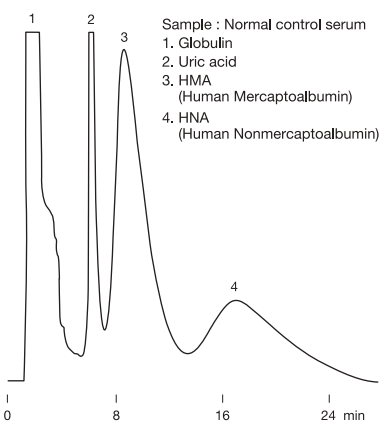

Sample : Normal control serum
 1. Globulin
 2. Uric acid
 3. HMA
 (Human Mercaptoalbumin)
 4. HNA
 (Human Nonmercaptoalbumin)

Column : Shodex Asahipak ES-502N 7C
Eluent : 50mM N-methylpiperazine-HCl
 buffer (pH4.8) + 400mM Na₂SO₄
 + 0.3% C₂H₅OH
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : 35°C


Nucleotides

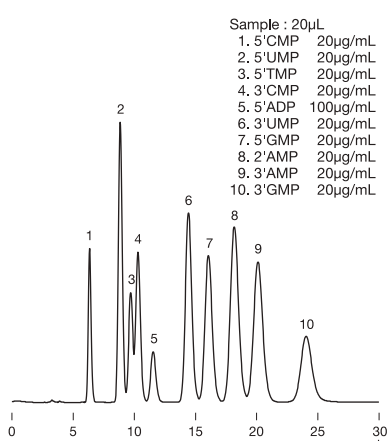

Sample : 20 μ L
 1. 5'UMP 20 μ g/mL
 2. 5'CMP 20 μ g/mL
 3. 5'TMP 20 μ g/mL
 4. 3'UMP 20 μ g/mL
 5. 3'ADP 100 μ g/mL
 6. 3'UMP 20 μ g/mL
 7. 5'GMP 20 μ g/mL
 8. 2'AMP 20 μ g/mL
 9. 3'AMP 20 μ g/mL
 10. 3'GMP 20 μ g/mL

Column : Shodex AXPak WA-624
Eluent : 0.35M CH₃COOH aq.
 /0.35M CH₃COONH₄ aq.=240/100
Flow rate : 1.0mL/min
Detector : UV (260nm)
Column temp. : 60°C

Sulfide ion and cyanide ion

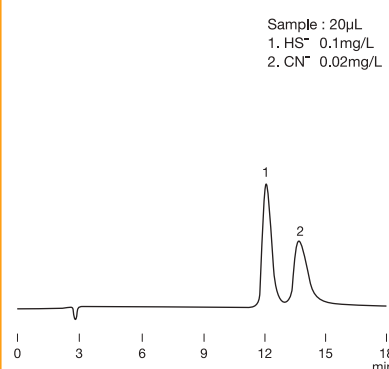

Sample : 20 μ L
 1. HS⁻ 0.1mg/L
 2. CN⁻ 0.02mg/L

Column : Shodex IEC DEAE-825
Eluent : 10mM Na₂CO₃
 + 1mM Ethylenediamine aq.
 + 10% CH₃OH
Flow rate : 1.0mL/min
Detector : Electrochemical
 (Electrode; Silver, 0mV SCE)
Column temp. : 25°C

Cation Exchange Chromatography Columns

Features

SP-825 CM-825	- Suitable for analyzing relatively high molecular weight compounds: proteins, peptides, DNA, and RNA - Usable in a wide pH range from pH 2 to 12
SP-420N	- Non-porous base material - For rapid analysis
New SP-FT 4A	- Non-porous base material - Provides ultra-rapid analysis using conventional devices
SP-2B	- Non-porous base material - Can be used with UHPLC (available under hyperbaric conditions for up to 30 MPa)
ES-502C 7C	- Compared to IEC series columns, polyvinyl alcohol is used as base material offering different separation pattern - Low hydrophobic interaction with proteins allows analysis under mild conditions
P-421S	- Column for amino acids analysis by cation exchange mode - Provides simultaneous analysis of different amino acids - Fulfills USP L22 and L58 requirements

Standard columns

[Strong cation exchange resin] Functional Group: Sulfopropyl

Product Code	Product Name	Ion Exchange Capacity (meq/g)	Base Material	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6118250	IEC SP-825	0.4	Polyhydroxymethacrylate	8	5,000	8.0 × 75	50mM Na ₂ SO ₄ aq.
F6113000	IEC SP-420N	0.3	Polyhydroxymethacrylate	2.5	–	4.6 × 35	20mM Sodium acetate buffer + 0.5M Na ₂ SO ₄ (pH5.0)
F6113100	New IEC SP-FT 4A	0.2	Polyhydroxymethacrylate	2.7	–	4.6 × 10	20mM *MES buffer (pH5.6)

Housing Material of SP-FT 4A: PEEK
*MES: 2-(N-Morpholino)ethanesulfonic acid

[Strong cation exchange resin] Functional Group: Sulfopropyl (UHPLC column)

Product Code	Product Name	Ion Exchange Capacity (meq/g)	Base Material	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6113110	PIKESS SP-2B	0.3	Polyhydroxymethacrylate	2.5	–	2.0 × 50	20mM Sodium acetate buffer + 0.5M Na ₂ SO ₄ (pH5.0)

[Weak cation exchange resin] Functional Group: Carboxymethyl

Product Code	Product Name	Ion Exchange Capacity (meq/g)	Base Material	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6110002	IEC CM-825	0.4	Polyhydroxymethacrylate	8	5,000	8.0 × 75	50mM Na ₂ SO ₄ aq.
F7640001	Asahipak ES-502C 7C	0.55	Polyvinyl alcohol	9	2,000	7.5 × 100	0.1M Sodium phosphate buffer (pH4.4)

[For amino acid analysis] Functional Group: Sulfo (Na⁺)


Product Code	Product Name	Plate Number (TP/column)	Base Material	Particle Size (μm)	Column Size (mm) I.D. x Length	Shipping Solvent
F6354211	CXpak P-421S	≥ 3,500	Styrene divinylbenzene copolymer	6	4.6 × 150	H ₂ O
F6700210	CXpak P-G	(guard column)	Styrene divinylbenzene copolymer	6	4.6 × 10	H ₂ O

Preparative columns *Preparative columns are made to order.


Product Code	Product Name	Particle Size (μm)	Column Size (mm) I.D. x Length	Standard column
F6548002	IEC SP-2025	20	20.0 × 150	SP-825
F6709604	IEC SP-G 8B (IEC SP-LG)	20	8.0 × 50	(guard column)
F6548003	IEC CM-2025	20	20.0 × 150	CM-825
F6709605	IEC CM-G 8B (IEC CM-LG)	20	8.0 × 50	(guard column)
F6840003	Asahipak ES-502C 20C	13	20.0 × 100	ES-502C 7C
F6710021	Asahipak GS-20G 7B	20	7.5 × 50	(guard column)

Protein separation using cation exchange columns


(I) CM-825
(Weak cation exchange)
90μL injection



(II) SP-825
(Strong cation exchange)
30μL injection



(III) SP-420N
(Strong cation exchange)
non-porous type gel



Column : (I) Shodex IEC CM-825, (II) Shodex IEC SP-825,
(III) Shodex IEC SP-420N

Eluent : (A); 20mM Sodium phosphate buffer (pH7.0)
(B); (A) + 0.5M NaCl

(I,II) Linear gradient; (A) to (B), 60min (III) Linear gradient; (A) to (B), 10min

Flow rate : (I,II) 1.0mL/min (III) 1.5mL/min

Detector : UV (280nm)


Column temp. : Room temp.

Sample :

1. Myoglobin
2. Trypsinogen
3. Ribonuclease A
4. α-Chymotrypsinogen A
5. Cytochrome c
6. Lysozyme

Ultra-rapid analysis of protein standards

Sample : 5μL
1. Trypsinogen 0.16%
2. α-Chymotrypsinogen A 0.08%
3. Ribonuclease A 0.12%
4. Cytochrome c 0.12%
5. Lysozyme 0.06%

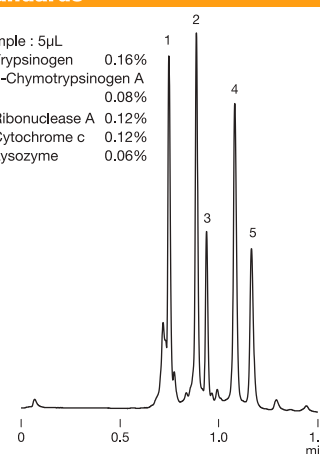

Column : Shodex IEC SP-FT 4A

Eluent : (A); 20mM MES buffer (pH5.6)
(B); (A) + 0.5M Na2SO4
Linear gradient; (A) to (B), 2min


Flow rate : 1.7mL/min

Detector : UV (280nm)

Column temp. : 30°C

Ultra-rapid analysis of hemoglobins

Sample : 5μL
AFSC Hemoglobin Control
(51-fold diluted)

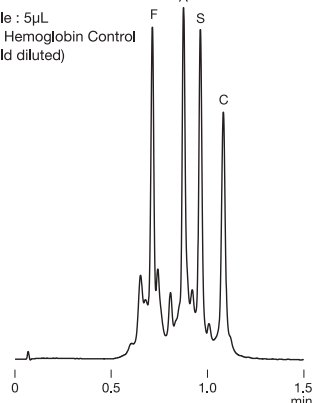

Column : Shodex IEC SP-FT 4A

Eluent : (A); 20mM MES buffer (pH5.6)
(B); (A) + 0.5M Na2SO4
Linear gradient;
5% (B) to 100% (B), 2min


Flow rate : 1.7mL/min

Detector : VIS (415nm)

Column temp. : 30°C

Analysis of nitrogen compounds following the testing methods for fertilizers

Sample : 10μg/mL each, 10μL
1. Urea
2. Biuret
3. Dicyandiamide
4. Guanidine
5. Guanilyurea

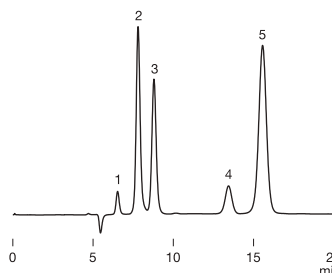

Column : Shodex Asahipak ES-502C 7C

Eluent : 3.92g KH2PO4 + 0.12g H3PO4
in 1000mL of H2O

Flow rate : 0.6mL/min


Detector : UV (190nm)

Column temp. : 40°C

Catecholamines

Sample : 300μg/mL each, 10μL

1. DOPA
Oc1ccc(cc1)CNC(=O)O
2. Adrenaline
Oc1ccc(cc1)CNC(C)O
3. Noradrenaline
Oc1ccc(cc1)CNC(O)O
4. Dopamine
Oc1ccc(cc1)CNCN

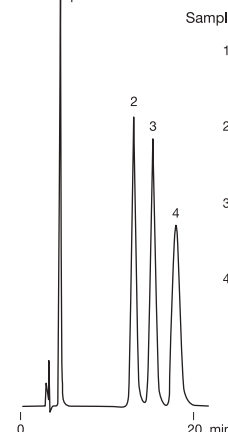

Column : Shodex Asahipak ES-502C 7C


Eluent : 20mM Sodium malonate buffer (pH6.0)
+ 0.5M NaCl

Flow rate : 1.0mL/min



Detector : UV (280nm)

Column temp. : 30°C

Paraquat and diquat



Sample : 20μL

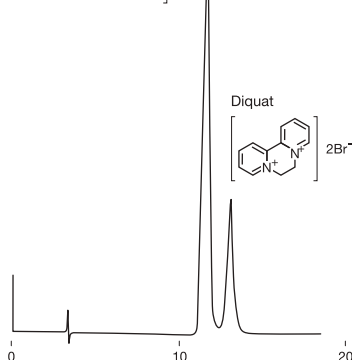

Column : Shodex Asahipak ES-502C 7C

Eluent : 50mM Sodium phosphate buffer (pH7.0)
+ 150mM NaCl

Flow rate : 1.0mL/min


Detector : UV (288nm)

Column temp. : 30°C

Standard amino acids

Sample : 0.1μM each, 100μL

1. Asp
2. Thr
3. Ser
4. Glu
5. Pro
6. Gly
7. Ala
8. Cys
9. Val
10. Met
11. Ile
12. Leu
13. Tyr
14. Phe
15. Lys
16. NH3
17. His
18. Arg

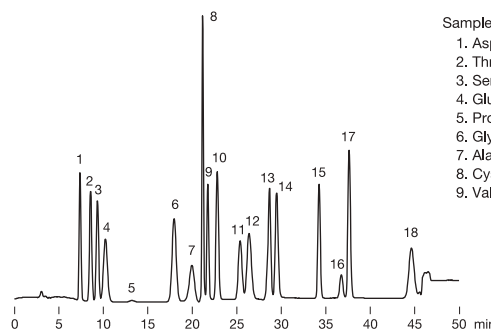

Column : Shodex CXpak P-421S

Eluent : MCI Buffer L-8500-PH Kit (Mitsubishi Chemical Corporation)
Low pressure gradient:
0min; PH-1, 0.2min; PH-2, 12.5min; PH-3, 22.7min; PH-4
40.0-53.0min; PH-RG

Reagent : Ninhydrin Coloring Solution Kit for HITACHI
(Wako Pure Chemical Industries, Ltd.)
0-52min; R1:R2=50:50

Flow rate : (Eluent) 0.5mL/min
(Reagent) 0.35mL/min

Detector : VIS (570nm)

Column Temp. : 63°C

Reaction Temp. : 120°C

Special Separation Modes Columns

Hydrophobic Interaction Chromatography Column

Features

- PH-814**
- Separates proteins without denaturation
 - Applicable to samples obtained after ammonium sulfate fraction treatment

Standard columns

Product Code	Product Name	Functional Group	Particle Size (µm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6110003	HIC PH-814	Phenyl	10	2,000	8.0 x 75	H ₂ O

Base Material: Polyhydroxymethacrylate

Affinity Chromatography Columns

Features

- AFpak**
- Rigid polymer-based packing materials enable high speed analysis
 - Functional group modified with chemically stable ligand (spacer)
 - Minimum detachment of functional groups ensures highly reproducible analysis

Standard columns

Product Code	Product Name	Ligand	Ligand Load/Gel (g)	Particle Size (µm)	Column Size (mm) I.D. x Length	Shipping Solvent
F7118946	AFpak APA-894	Protein A	4mg	18	8.0 x 50	0.1M Sodium phosphate buffer + 0.5M NaCl + 0.02% NaN ₃ (pH7.0)
F7118964	AFpak ACH-494	Choline oxydase, Acetylcholine esterase	–	18	4.6 x 10	10mM Sodium Phosphate buffer + 1.0M NaCl (pH7.4)

Base Material: Polyhydroxymethacrylate

Chiral Separation Columns

Features

- CDBS-453**
- Separates optical isomers by using their conformational compatibility differences
 - Versatile column for chiral separation
 - Fulfills USP L45 requirements

- CRX-853**
- Separates optical isomers by using their differences in metal complex formation capacities
 - Suitable for amino acids, hydroxyl acids, and their derivatives

Standard columns

Product Code	Product Name	Functional Group	Base Material	Particle Size (µm)	Column Size (mm) I.D. x Length	Shipping Solvent
F7146003	ORpak CDBS-453	β -Cyclodextrin derivative	Silica	3	4.6 x 150	1.0% CH ₃ COOH + 0.2M NaCl aq. /CH ₃ CN=70/30
F7140040	ORpak CRX-853	L-Amino acid derivative	Polyhydroxymethacrylate	6	8.0 x 50	0.25mM CuSO ₄ aq.
F6709300	ORpak CRX-G	(guard column)	Polyhydroxymethacrylate	6	4.6 x 10	0.25mM CuSO ₄ aq.

High Temperature Reversed Phase Chromatography Column

Features

- ET-RP1**
- Capable of high temperature analysis up to 150°C
 - High temperature analysis improves column efficiency and enables rapid analysis
 - Fulfills USP L67 requirements

Standard columns

Product Code	Product Name	Plate Number (TP/column)	Functional Group	Particle Size (µm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F7623001	ET-RP1 4D	≥ 11,000	Octadecyl	4	250	4.6 x 150	H ₂ O/CH ₃ CN=35/65

Base Material: Polyvinyl alcohol

Pretreatment Column for Column Switching Method

Feature


- GF-4A**
- Higher protein removal rate

Column for column switching method

Product Code	Product Name	Particle Size (µm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F8700015	MSpak GF-4A	9	400	4.6 x 10	H ₂ O

Base Material: Polyvinyl alcohol


Protein separation by hydrophobic interaction chromatography

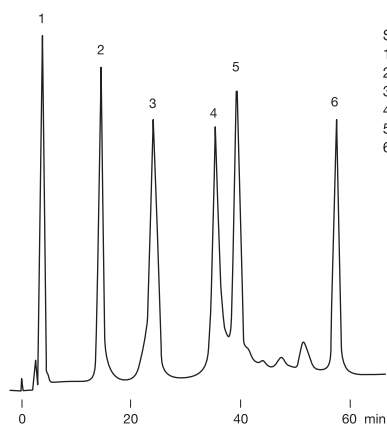

Sample : 370µL
 1. Cytochrome c 0.03%
 2. Myoglobin 0.08%
 3. Ribonuclease A 0.16%
 4. Ovalbumin 0.16%
 5. Lysozyme 0.04%
 6. α-Chymotrypsinogen 0.05%

Column : Shodex HIC PH-814
Eluent : (A); 1.8M Ammonium sulfate + (B)
 (B); 0.1M Phosphate buffer (pH7.0)
 Linear gradient; (A) to (B), 60min
Flow rate : 1.0mL/min
Detector : UV (280nm)
Column temp. : Room temp.

Choline and acetylcholine

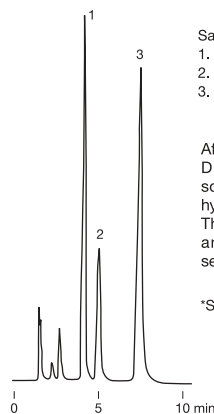


Sample : 10µL
 1. Choline 5mg/L
 2. Ethylthiomocholine 10mg/L
 3. Acetylcholine 10mg/L

After choline and acetylcholine are separated using DE-413 polymer-based reversed phase column, solutes are passed through ACH-494 to generate hydrogen peroxide. The resulting hydrogen peroxide is detected using an electrochemical detector to enable highly sensitive analysis.

*See page 12 for DE-413

Column : Shodex RSpak DE-413
Post column : Shodex AFpak ACH-494
Eluent : 0.1M H₃PO₄ + 300mg/L Sodium 1-decansulfonate +
 65mg/L Tetramethylammonium chloride
 (pH8.0 adjusted by 1.0M NaOH)
Flow rate : 1.0mL/min
Detector : Electrochemical (Electrode : Pt, 350mV SCE)
Column temp. : 37°C


Chiral separation of epinephrines

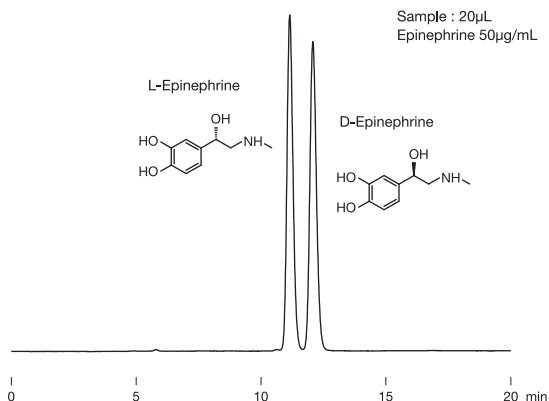

Sample : 20µL
 Epinephrine 50µg/mL

Column : Shodex ORpak CDBS-453
Eluent : (0.05% (w/v) CH₃COOH + 0.2M NaCl) aq./CH₃CN=95/5
Flow rate : 0.5mL/min
Detector : UV (280nm)
Column temp. : 10°C


Chiral separation of lactic acids

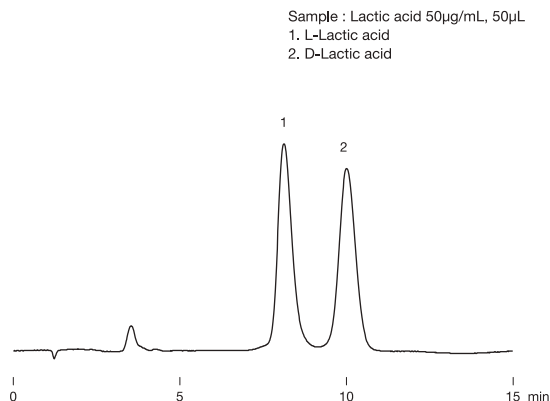

Sample : Lactic acid 50µg/mL, 50µL
 1. L-Lactic acid
 2. D-Lactic acid

Column : Shodex ORpak CRX-853
Eluent : 0.5mM CuSO₄ aq.
Flow rate : 1.0mL/min
Detector : UV (230nm)
Column temp. : 50°C

Chiral separation of mandelic acids

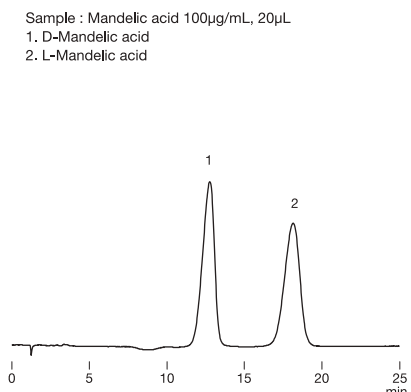


Sample : Mandelic acid 100µg/mL, 20µL
 1. D-Mandelic acid
 2. L-Mandelic acid

Column : Shodex ORpak CRX-853
Eluent : 0.25mM CuSO₄ aq.
Flow rate : 1.0mL/min
Detector : UV (230nm)
Column temp. : 50°C

Comparison of ET-RP1's column efficiencies (theoretical plate height) observed at high and normal temperature conditions

high temp. (150°C)
 2.4mL/min

normal temp. (40°C)
 0.5mL/min



Sample :
 1. Uracil
 2. Pyridine
 3. Acetophenone
 4. Benzene

Sample	Reduced plate height *	
	40°C	150°C
Acetophenone	3.2	2.4
Benzene	3.6	2.3

* Plate height / particle diameter of the packed resin

Column : Shodex ET-RP1 4D
Eluent : (Left) H₂O/CH₃CN=50/50
 (Right) H₂O/CH₃CN=75/25
Detector : Photodiode array (210nm)
Column Oven : Polaratherm 9000 Series
 (SandraSclerity Technologies, Inc)

Note:
 The eluent was introduced into the column after being preheated and was cooled after column elution, then introduced into the detector.

Data provided by Research Institute for Chromatography bvba

● GPC Clean-up Columns


Features

EV

- Suitable for fractionation of residual pesticides in foods
- EV-2000 AC is used in Shoku-An No. 1003001 (October 3rd, 2006, Japan) of the Pharmaceutical and Food Safety Bureau, MHLW, Section 2 “Simultaneous GC/MS (LC/MS) Analyses of Agricultural Chemicals in Livestock and Marine Products”.
- EV2000AC-12F is used in Shoku-An No. 0226 (February 26th, 2015, Japan) of the Pharmaceutical and Food Safety Bureau, MHLW, Section 2 “LC/MS Analyses of Agricultural Chemicals in Livestock and Marine Products”.

PAE

- Suitable for cleaning up high-moisture samples such as blood and bottom sediment
- Highly effective for fractionation of endocrine disruptors in environmental samples

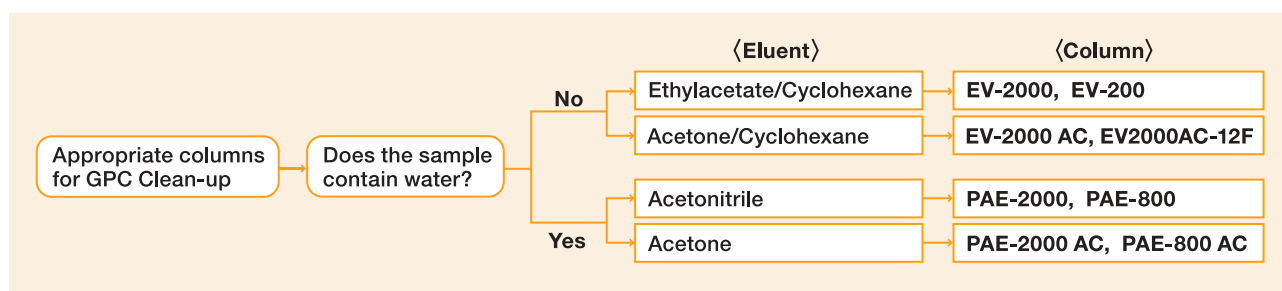

■ GPC Clean-up for residual pesticides in foods, etc.

Product Code	Product Name	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6090006	CLNpak EV2000AC-12F	16	30	12.0 × 300	Acetone/Cyclohexane=3/7
F6090007	CLNpak EV-G AC12C	16	(guard column)	12.0 × 100	Acetone/Cyclohexane=3/7
F6090003	CLNpak EV-2000 AC	16	30	20.0 × 300	Acetone/Cyclohexane=3/7
F6090004	CLNpak EV-G AC	16	(guard column)	20.0 × 100	Acetone/Cyclohexane=3/7
F6090001	CLNpak EV-2000	16	30	20.0 × 300	Ethylacetate/Cyclohexane=3/7
F6090002	CLNpak EV-G	16	(guard column)	20.0 × 100	Ethylacetate/Cyclohexane=3/7
F6090005	CLNpak EV-200	16	30	2.0 × 150	Ethylacetate/Cyclohexane=3/7

Base Material: Styrene divinylbenzene copolymer


■ GPC Clean-up for phthalic acid esters in sediments, biological samples, blood, etc.

Product Code	Product Name	Particle Size (μm)	Pore Size (Å)	Column Size (mm) I.D. x Length	Shipping Solvent
F6810022	CLNpak PAE-2000	5	400	20.0 × 300	Acetonitrile
F6714007	CLNpak PAE-G	9	(guard column)	8.0 × 50	Acetonitrile
F7600025	CLNpak PAE-800	5	400	8.0 × 300	Acetonitrile
F6810023	CLNpak PAE-2000 AC	5	400	20.0 × 300	Acetone
F6714008	CLNpak PAE-G AC	9	(guard column)	8.0 × 50	Acetone
F7600026	CLNpak PAE-800 AC	5	400	8.0 × 300	Acetone

Base Material: Polyvinyl alcohol


Sample preparation outline for simultaneous GC/MS and LC/MS analysis of agricultural chemicals in livestock and marine products (part 1)

[Outline]

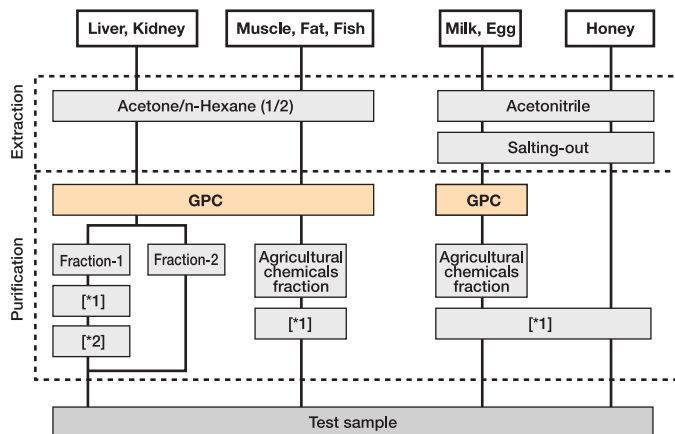

GPC column : Shodex CLNpak EV-2000 AC + EV-G AC
 *1 Purification with ethylenediamine-N-propylsilylated silica gel mini-column
 *2 Purification with silica gel mini-column


Preparation range of agricultural chemicals using EV-2000 AC

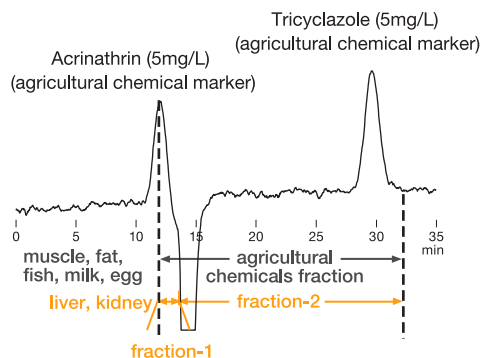

Column : Shodex CLNpak EV-G AC + EV-2000 AC
 Eluent : Acetone/Cyclohexane=1/4
 Flow rate : 5.0mL/min
 Detector : UV (254nm)
 Column temp. : 40°C
 Injection vol. : 5mL


Sample preparation outline for simultaneous LC/MS analysis of agricultural chemicals in livestock and marine products (part 2)

[Outline]

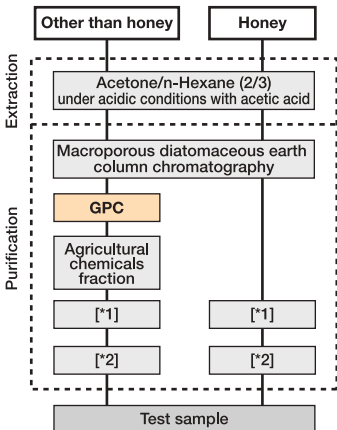


GPC column : Shodex CLNpak EV2000AC-12F + EV-G AC12C
 *1 Purification with trimethyl aminopropylsilylated silica gel mini-column
 *2 Purification with ethylenediamine-N-propylsilylated silica gel mini-column

Preparation range of agricultural chemicals using EV2000AC-12F

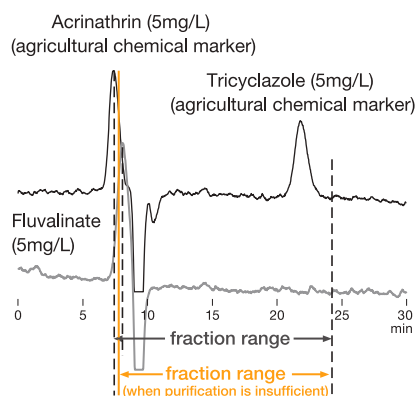


Column : Shodex CLNpak EV-G AC12C + EV2000AC-12F
 Eluent : Acetone/Cyclohexane=3/17
 Flow rate : 3.0mL/min
 Detector : UV (254nm)
 Column temp. : 45°C
 Injection vol. : 2mL

GPC Clean-up of fatty tuna and beef tallow

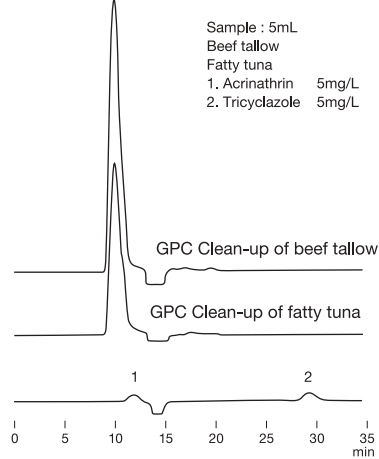

Column : Shodex CLNpak EV-G AC + EV-2000 AC
 Eluent : Acetone/Cyclohexane=1/4
 Flow rate : 5.0mL/min
 Detector : UV (254nm)
 Column temp. : 40°C
 Injection vol. : 5mL


Separation of PSB and insulating oil using PAE-800

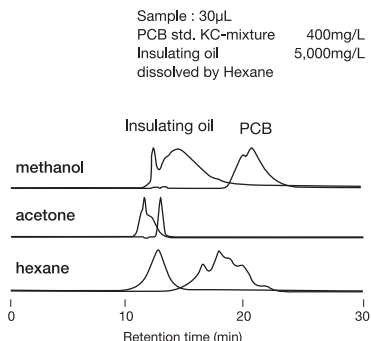

Column : Shodex CLNpak PAE-800
 Eluent : Methanol, Acetone, Hexane
 Flow rate : 0.8mL/min
 Detector : Photodiode array (209nm)
 Column temp. : 40°C


Source: Mr. Tetsuya Sawatsubashi (Mitsubishi Heavy Industries, Ltd.) et al., Search of Liquid Chromatographic Clean-up Materials for Rapid PCB Analysis and Evaluation of Their Separation Characteristics. Journal of Environmental Chemistry, 2007, Vol. 17, No. 3, p. 471-481.

GPC Clean-up of carcinogens in diesel dust measured using PAE-800 AC

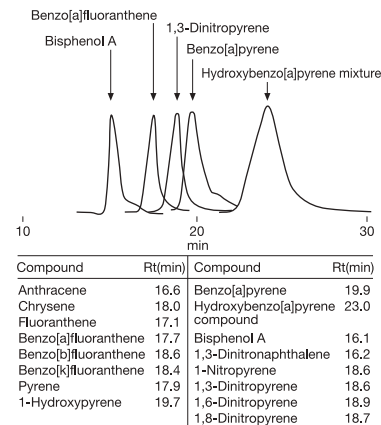

Column : Shodex CLNpak PAE-800 AC
 Eluent : Acetone
 Flow rate : 0.8mL/min
 Detector : UV (210nm)
 Column temp. : Room temp.
 Data provided by Kazuichi Hayakawa Ph.D., Faculty of Pharmaceutical Sciences, Kanazawa University.

Eluting positions of phthalic acid esters using PAE-800 AC

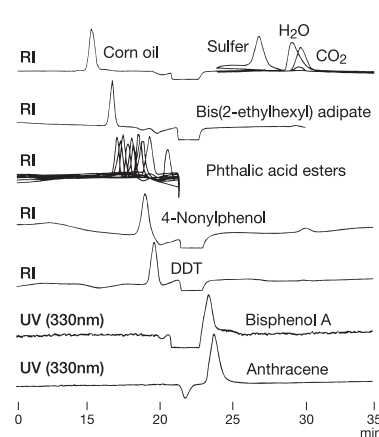

Column : Shodex CLNpak PAE-800 AC
 Eluent : Acetone
 Flow rate : 0.5mL/min
 Detector : UV (330nm), RI
 Column temp. : Room temp.

● Product Name Changes Notices

Some Shodex guard columns have been renamed.
There is no change in their product codes.

■ Renamed products list

Page	New Product Name	Former Product Name	Product Code
12	RSpak DE-G 4A	RSpak DE-G	F6700150
12	RSpak DE-G 2A	RSpak DE-SG	F6700151
12	RSpak DM-G 4A	RSpak DM-G	F6700160
13	RSpak DE-G 8B	RSpak DE-LG	F6700190
13	RSpak DM-G 8B	RSpak DM-LG	F6700404
26	SUGAR SC-G 6B	SUGAR SC-LG	F6700090
26	SUGAR SP-G 6B	SUGAR SP-G	F6700081
26	SUGAR KS-G 6B	SUGAR KS-G	F6700020
26	RSpak DC-G 4A	RSpak DC-G	F6700170
26	SUGAR SC1211G 4A	SUGAR SC-G	F6700120
27	SUGAR KS-G 8B	SUGAR KS-LG	F6700002
27	RSpak DC-G 8B	RSpak DC-LG	F6700402
30	RSpak KC-G 6B	RSpak KC-G	F6700030
30	RSpak KC-G 8B	RSpak KC-LG	F6700010
38	PROTEIN KW-G 6B	PROTEIN KW-G	F6700131
39	PROTEIN KW-G 8B	PROTEIN KW-LG	F6709556
42	OHpak SB-G 6B	OHpak SB-G	F6709430
43	OHpak SB-G 8B	OHpak SB-LG	F6709555
50, 56	GPC KF-G 4A	GPC KF-G	F6700300
52	GPC K-G 4A	GPC K-G	F6700401
54	GPC KD-G 4A	GPC KD-G	F6700411
60	GPC KF-G 8B	GPC KF-LG	F6700406
60	GPC K-G 8B	GPC K-LG	F6700407
61	GPC H-G 8B	GPC H-G	F6700310
61	GPC KF-G 20C	GPC KF-LLG	F6700408
61	GPC K-G 20C	GPC K-LLG	F6700409
68	GPC HFIP-G 8B	GPC HFIP-LG	F6700500
68	GPC HFIP-G 4A	GPC HFIP-G	F6700511
70	IEC QA-G 8B	IEC QA-LG	F6709602
70	IEC DEAE-G 8B	IEC DEAE-LG	F6709603
72	IEC SP-G 8B	IEC SP-LG	F6709604
72	IEC CM-G 8B	IEC CM-LG	F6709605

USP40-NF35 Column List

No.	Packing Material	Recommended Column	Page
L1	Octadecyl silane chemically bonded to porous or non-porous silica or ceramic micro-particles, 1.5 to 10µm in diameter, or a monolithic rod.	C18	22
		Silica C18M	22
		Silica C18P	22
L3	Porous silica particles, 1.5 to 10µm in diameter, or a monolithic silica rod.	Silica 5SIL	23
L7	Octylsilane chemically bonded to totally or superficially porous silica particles, 1.5 to 10µm in diameter, or a monolithic silica rod.	Silica 5C8	22
L8	An essentially monomolecular layer of aminopropylsilane chemically bonded to totally porous silica gel support, 1.5-10µm in diameter, or a monolithic silica rod.	Silica 5NH	23
L10	Nitrile groups chemically bonded to porous silica particles, 1.5-10µm in diameter, or a monolithic silica rod.	Silica 5CN	22
L11	Phenyl groups chemically bonded to porous silica particles, 1.5-10µm in diameter, or a monolithic silica rod.	Silica 5NPE	22
L17	Strong cation-exchange resin consisting of sulfonated cross-linked styrene-divinylbenzene copolymer in the hydrogen form, 6 to 12µm in diameter.	SUGAR SH1011	30
		SUGAR SH1821	30
		RSpak KC-811	30
		IC Y-521	34
L19	Strong cation-exchange resin consisting of sulfonated cross-linked styrene-divinylbenzene copolymer in the calcium form, about 5-15µm in diameter.	SUGAR SC1011	26
		SUGAR SC1821	26
		SUGAR SC1211	26
		EP SC1011-7F	27
		USPpak MN-431	27
		PROTEIN KW-800 series	38
L20	Dihydroxypropane groups chemically bonded to porous silica or hybrid particles, 1.5-10µm in diameter, or a monolithic silica rod.	PROTEIN LW-803	38
		KW400 series	38
		RSpak RP18-415	12
L21	A rigid, spherical styrene-divinylbenzene copolymer, 3 to 30µm in diameter.	RSpak DS-613	12
		RSpak DS-413	12
		GPC KF, K, KD, HK, LF, HT, UT, AT, HFIP series	50,52,54,56 58,62,64,66
		SUGAR SC1011	26
L22	A cation-exchange resin made of porous polystyrene gel with sulfonic acid groups, about 5-15µm in diameter.	SUGAR SC1821	26
		SUGAR SP0810	26
		SUGAR KS-800 series	26
		RSpak DC-613	26
		SUGAR SZ5532	26
		SUGAR SC1211	26
		EP SC1011-7F	27
		USPpak MN-431	27
		SUGAR SH1011	30
		SUGAR SH1821	30
		RSpak KC-811	30
		IC Y-521	34
		CXpak P-421S	72
		IEC QA-825	70
L23	An anion-exchange resin made of porous polymethacrylate or polyacrylate gel with quaternary ammonium groups, 7-12µm in size.	OHpak SB-802 HQ	42
		OHpak SB-802.5 HQ	42
L25	Packing having the capacity to separate compounds with a molecular weight range from 100-5000 (as determined by polyethylene oxide), applied to neutral, anionic, and cationic water-soluble polymers. A polymethacrylate resin base, cross-linked with polyhydroxylated ether (surface contained some residual carboxyl functional groups) was found suitable.	PROTEIN KW-800 series	38
		PROTEIN LW-803	38
		KW400 series	38
L33	Packing having the capacity to separate dextrans by molecular size over a range of 4,000 to 500,000 Da. It is spherical, silica-based, and processed to provide pH stability.	SUGAR SP0810	26
L34	Strong cation-exchange resin consisting of sulfonated cross-linked styrene-divinylbenzene copolymer in the lead form, about 7 to 9µm in diameter.	OHpak SB-803 HQ	42
L37	Packing having the capacity to separate proteins by molecular size over a range of 2,000 to 40,000 Da. It is a polymethacrylate gel.	OHpak LB-803	42
L38	A methacrylate-based size-exclusion packing for water-soluble samples.	OHpak SB-800 HQ series	42
		OHpak LB-800 series	42
		ODP2 HP	8
		RSpak DM-614	12
L39	A hydrophilic polyhydroxymethacrylate gel of totally porous spherical resin.	OHpak SB-800 HQ series	42
		OHpak LB-800 series	42
		ORpak CDBS-453	74
L45	Beta cyclodextrin, R,S-hydroxypropyl ether derivative, bonded to porous silica particles, 3-10µm in diameter.	RSpak DC-613	26
L58	Strong cation-exchange resin consisting of sulfonated cross-linked styrene-divinylbenzene copolymer in the sodium form, about 6 to 30µm in diameter.	SUGAR KS-800 series	26
		CXpak P-421S	72
		PROTEIN KW-800 series	38
L59	Packing for the size-exclusion separations of proteins (separation by molecular weight) over the range of 5 to 7000 kDa. The packing is a spherical 1.5- to 10-µm, silica or hybrid packing with a hydrophilic coating.	PROTEIN LW-803	38
		KW400 series	38
		Asahipak ODP-40	10
L67	Porous vinyl alcohol copolymer with a C18 alkyl group attached to the hydroxyl group of the polymer, 2 to 10µm in diameter.	Asahipak ODP-50	10
		ET-RP1	74
		RSpak DE-613	12
L71	A rigid, spherical polymetacrylate, 4 to 6µm in diameter.	RSpak DE-413	12
		RSpak DE-213	12
		IC YK-421	34
L76	Silica-based, weak cation-exchange material, 5 µm in diameter. Substrate is surface polymerized polybutadiene-maleic acid to provide carboxylic acid functionalities. Capacity not less than 29µEq/column.	Asahipak NH2P-50	20
L82	Polyamine chemically bonded to cross-linked polyvinyl alcohol polymer, 5µm in diameter.		

Column Cleaning Procedures

Change in peak shapes, elution timing, and the elevated column pressure may be resolved by cleaning the column. This section describes general indications of column deterioration and column cleaning procedures. For detailed column cleaning procedures, refer to operating manual packaged with each column.

Typical indicators of column deterioration

1. Elevated column pressure
2. Abnormal peak shapes (broadening, leading, or tailing) and split peaks
3. Change in retention time
4. Unstable baseline

Cleaning solvent selection guide

Solvents capable of dissolving the adsorbed substances

Solvents with high eluting power (variable depending on separation mode)

***Use the solvent specified in the operation manual.**

Standard cleaning procedures

For an efficient cleaning, reverse the direction and reduce the flow rate to 1/3 of the regular flow.

Reversed phase chromatography columns	Clean the columns with solvent containing higher concentration of organic solvent such as methanol, acetonitrile, or THF. (In case of using buffer as a mobile phase, miscibility of the buffer solution and the organic solvents need to be checked)
Sugar analysis columns	[Ligand exchange columns (SUGAR series)] • In case of counter ion detachment Flush or inject solvent containing the salt corresponding to the modified counter-ligand. [Polymer-base amino columns (NH2P series)] • In cases where an acidic substance has been bound to the amino functional group Flush with solvents in the following sequence: water, 0.1M perchloric acid (aq.), water, 0.1M NaOH (aq.), water, and mobile phase.
Aqueous SEC (GFC) chromatography columns	• In cases where an ionic substance has been adsorbed Use a solvent with higher salt concentration or solvent with different pH from the mobile phase. • In cases where a hydrophobic substance has been adsorbed Use a solvent containing organic solvent. (In case of using buffer as a mobile phase, miscibility of the buffer solution and the organic solvents need to be checked)
Ion exchange chromatography columns	• In cases where an ionic substance has been adsorbed Use a solvent with higher salt concentration or solvent with different pH from the mobile phase. • In cases where a hydrophobic substance has been adsorbed Use a solvent containing organic solvent. (In case of using buffer as a mobile phase, miscibility of the buffer solution and the organic solvents need to be checked) • In cases where protein have been adsorbed Inject 1-2 mL of 0.1 M NaOH (aq.) or 30% (v/v) acetic acid (aq.) several times.
Hydrophobic interaction chromatography columns	• In cases where protein have been adsorbed Inject 1-2 mL of 0.1 M NaOH (aq.) or 30% (v/v) acetic acid (aq.) several times.

*The volume of the cleaning solvent required is 5-10 times the column volume.

*Avoid pressure elevation during the cleaning.

*The cleaning is limited and does not guarantee the full regeneration of the column to its original condition.

For your information

One typical cause of the column pressure elevation is the solid substance being clogged at the inlet filter of the column. In this case, reverse the direction and reduce the flow to 1/3 of the regular flow rate. This may remove the solid substance causing the elevated pressure.

● General Precautions for Column Handling

For the best performance of the column, please follow the instructions given below.

■ Column mounting

- Before mounting the column, replace the eluent within all the HPLC system with the mobile phase used for the analysis. *If the mobile phase of the choice is not miscible with the eluent already in the system, use solvent that is miscible with both solvents first to clean the system. *Buffer or salt solution may precipitate when mixed with organic solvent of different concentrations.
- Attach the column in the direction as indicated by arrow marked on the column. Gradually increase the flow rate of the solvent introduced to the column.
- When heating the column, be sure to pump the eluent at a low flow rate until the specified temperature is reached, and then gradually increase the flow rate up to the requirement after the column has been heated sufficiently.

■ Column dismounting

- If the column is heated, turn off the heater while keeping the flow rate at 1/3 of the regular flow.
- Turn off the pump when the column is cooled to room temperature.
- Remove the column from the system securely tighten the end caps.

■ Column storage

- For long-term storage, replace the solvent with shipping solvent and securely tighten the end caps.
- Store the column in a location with stable temperature.
- For long-term storage of SEC columns, immersion method is recommended.
*Please refer to the immersion method on the operation manual.

■ Other

- Avoid physical shock on the column. Be cautious not to drop the column from a high position.
- Do not bend the column.
- Avoid opening the column's end-fitting, it can cause alteration of column's performance.


*Read the operation manual before using the column.

Column Trouble Shooting


Common causes for abnormal chromatograms

Abnormal peak shapes

□Main cause □Solution ■Frequent problem

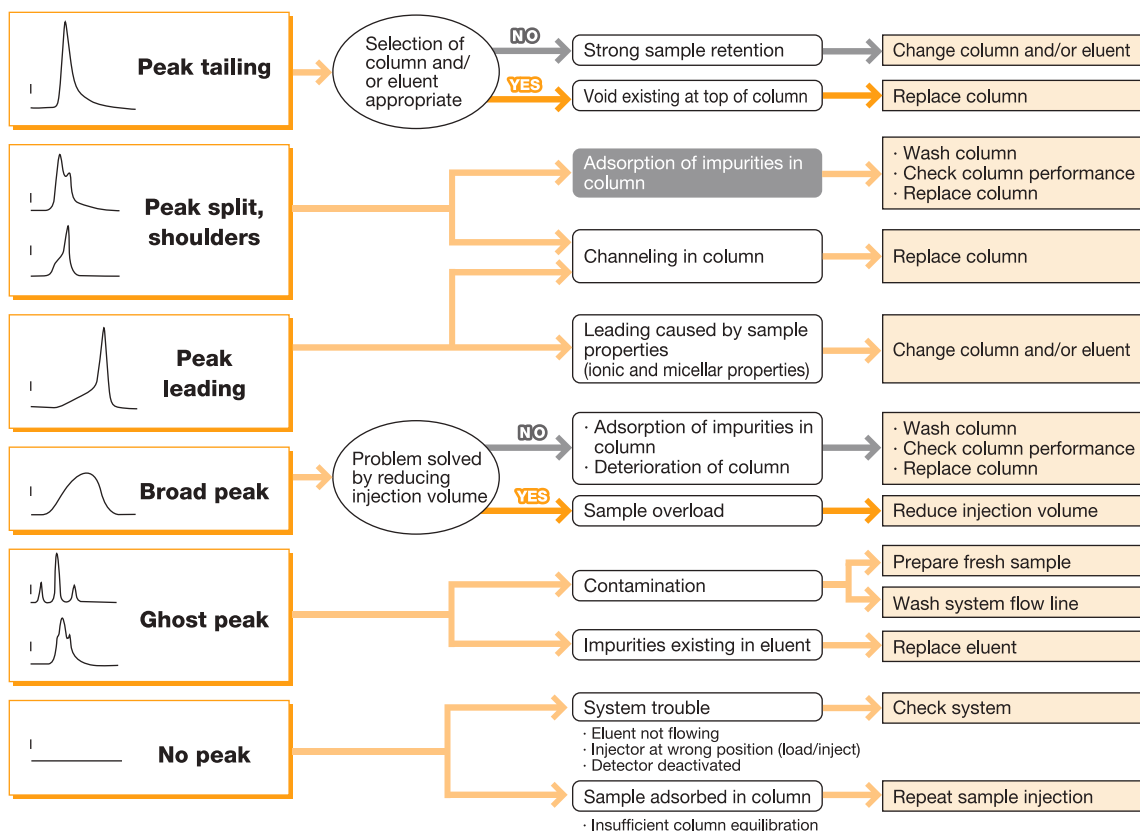


Pressure elevation

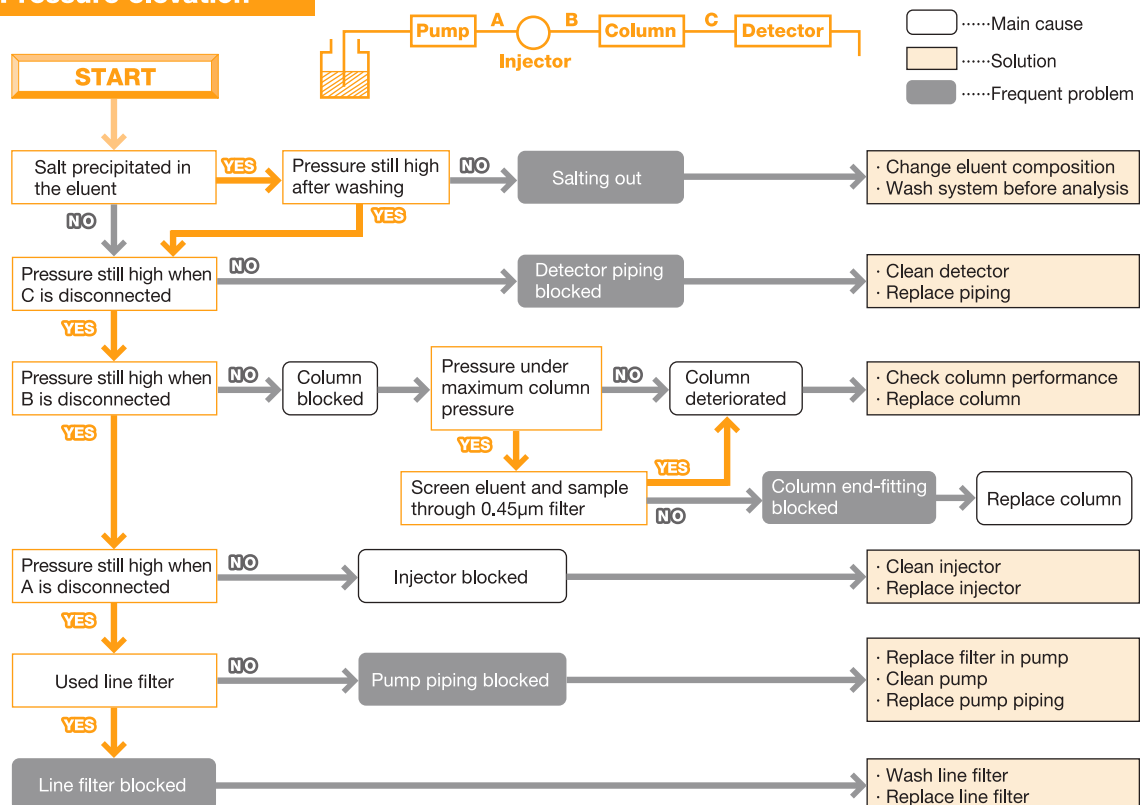


HPLC System Trouble Shooting

Common causes for abnormal chromatograms

Unstable baseline

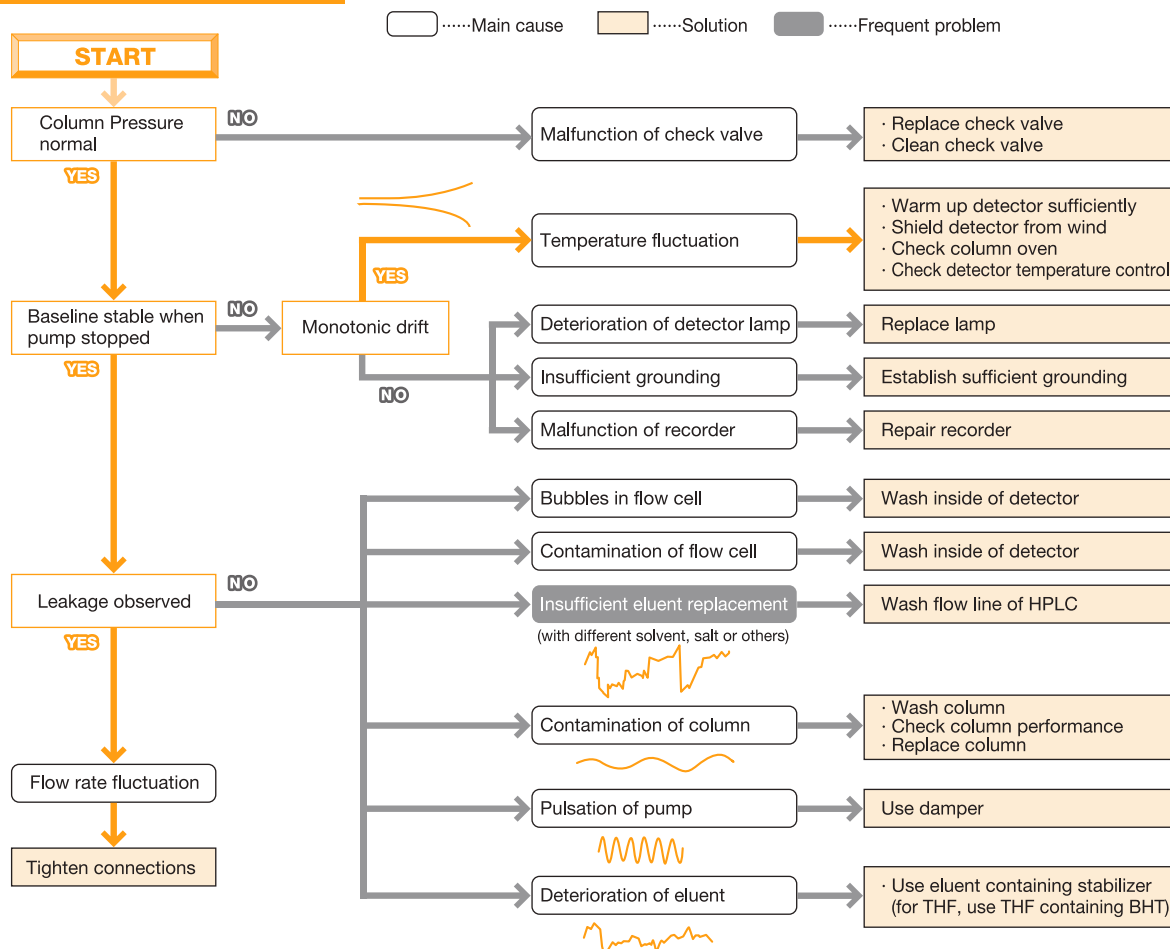

Noise

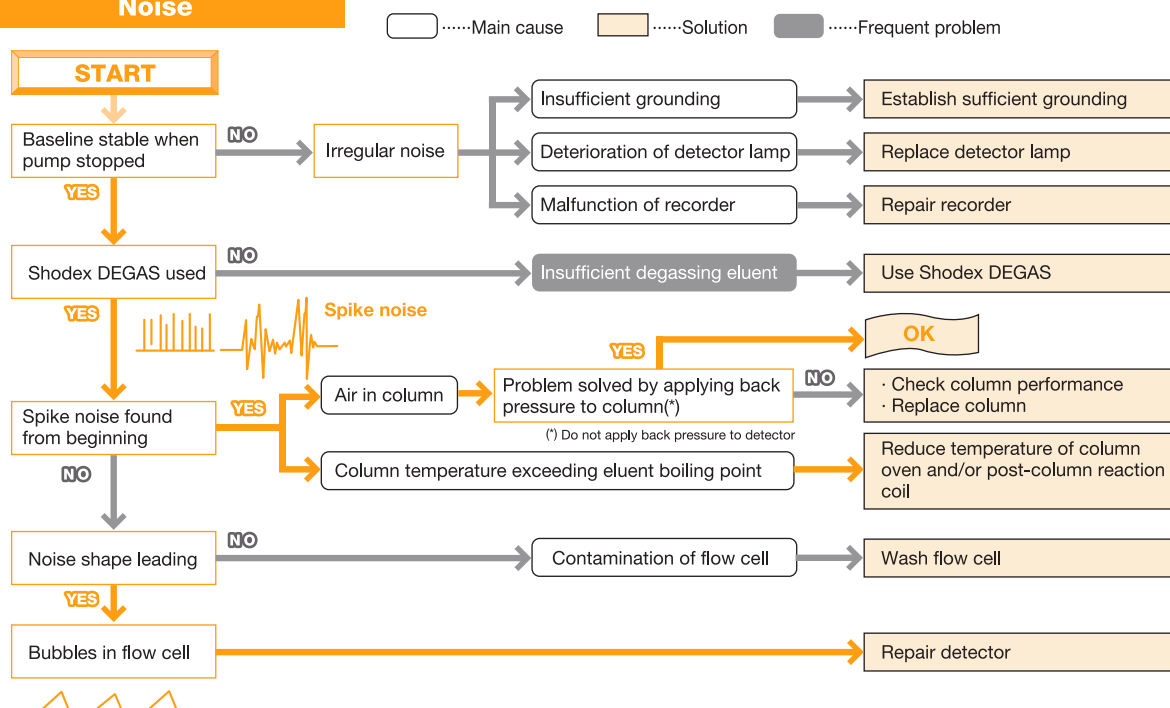

Index by Product Name

Columns are listed in alphabetical order without their series names.

[Series name]

AFpak	Asahipak	AXpak	CLNpak	CXpak	EP	GPC	HIC
HILICpak	IC	IEC	MSpak	OHpak	ORpak	PIKESS	PROTEIN
RSpak	Silica	STANDARD	STD	SUGAR	USPpak		

A

ACH-494	74
APA-894	74
AT-806MS	64

C

C18	22
C18M	22
C18P	22
C4P-50	10
5C8	22
C8P-50	10
CDBS-453	74
CM	72
5CN	22
CRX-853	74

D

DC	26, 27
DE	12, 13
DEAE	70
DM	12, 13
DS	12

E

ET-RP1 4D	74
ES-502C	72
ES-502N	70
EV	76

F

FL-1, FL-1 filter	32, 34
-------------------	--------

G

GF-210	48
GF-310	48
GF-4A	74
GF-510	48
GF-710	48
GF-7M HQ	48
GS-220	46
GS-310	48
GS-320	46
GS-510	48
GS-520	46
GS-620	46
GS-710	48
GSM-700	48

H

H-2000	61
HFIP-600	66
HFIP-800	66
HK-400	58
HK-HFIP404L	58
HT-800	64

I

I-524A	32
--------	----

J

JJ-50	12
-------	----

K

K-2000	60
K-5000	61
K-800	52
K-800D	52, 54
KC	30
KD-800	54
KF-2000	60
KF-5000	61
KF-400HQ	56
KF-600	56
KF-800D	50, 54
KF-800	50
KS-2000	27
KS-800	26
KW400	38
KW-800	38
KW-2000	39

L

LB-800	42
LF	62
LW-803	38

M

M-75	69
MN-431	27

N

5NH	23
NH2P	20
NI-424	32
NN	12, 13
5NPE 4D	22

O

ODP2 HP	8
ODP	10

P

P-421S	72
P-82	69
P	69
PAE	76
PH-814	74
5PYE 4D	22

Q

QA-825	70
--------	----

R

RP18-415	12
----------	----

S

SB-2000	43
SB-800 HQ	42
SC1011, SC1821	26
SC1011-7F	27
SC1211	26
SH1011, SH1821	30
SH-75	69
SI-35	32
SI-50 4E	32
SI-52 4E	32
SI-90 4E	32
5SIL	23
SL-105	69
SM-105	69
SP0810	26
SP	72
SZ5532	26

T

T-521	34
-------	----

U

UT-800	64
--------	----

V

VC-50	16
VG-50	16
VN-50	16
VT-50	16

W

WA-624	70
--------	----

Y

Y-521	34
YK-421	34
YS-50	34

● Index by Product Code

Product Code	Product Name	Page
F6021030	HFIP-603	66
F6021040	HFIP-604	66
F6021041	LF-804	62
F6021042	LF-604	62
F6021043	LF-404	62
F6021050	HFIP-605	66
F6021060	HFIP-606	66
F6021070	HFIP-607	66
F6021080	HFIP-606M	66
F6025010	HK-401	58
F6025050	HK-405	58
F6026040	HK-404L	58
F6026140	HK-HFIP404L	58
F6027030	KF-803L	50
F6027040	KF-804L	50
F6027050	KF-805L	50
F6027060	KF-806L	50
F6027070	KF-807L	50
F6028010	KF-801	50
F6028020	KF-802	50
F6028025	KF-802.5	50
F6028030	KF-803	50
F6028040	KF-804	50
F6028050	KF-805	50
F6028060	KF-806	50
F6028070	KF-807	50
F6028090	KF-806M	50
F6028091	KF-601	56
F6028092	KF-602	56
F6028093	KF-602.5	56
F6028094	KF-603	56
F6028095	KF-604	56
F6028096	KF-605	56
F6028097	KF-606	56
F6028098	KF-606M	56
F6028099	KF-607	56
F6028110	K-801	52
F6028111	KF-401HQ	56
F6028112	KF-402HQ	56
F6028114	KF-402.5HQ	56
F6028116	KF-403HQ	56
F6028118	KF-404HQ	56
F6028119	KF-405LHQ	56
F6028120	K-802	52
F6028122	KF-406LHQ	56
F6028125	K-802.5	52
F6028130	K-803	52
F6028140	K-804	52
F6028150	K-805	52
F6028160	K-806	52
F6028170	K-807	52
F6028190	K-806M	52
F6028194	K-803L	52
F6028195	K-804L	52
F6028196	K-805L	52

Product Code	Product Name	Page
F6028197	K-806L	52
F6028198	K-807L	52
F6028210	KD-801	54
F6028220	KD-802	54
F6028225	KD-802.5	54
F6028230	KD-803	54
F6028240	KD-804	54
F6028250	KD-805	54
F6028260	KD-806	54
F6028270	KD-807	54
F6028290	KD-806M	54
F6028530	HFIP-803	66
F6028540	HFIP-804	66
F6028550	HFIP-805	66
F6028560	HFIP-806	66
F6028570	HFIP-807	66
F6028590	HFIP-806M	66
F6090001	EV-2000	76
F6090002	EV-G	76
F6090003	EV-2000 AC	76
F6090004	EV-G AC	76
F6090005	EV-200	76
F6090006	EV2000AC-12F	76
F6090007	EV-G AC12C	76
F6102001	H-2001	61
F6102002	H-2002	61
F6102003	H-2003	61
F6102004	H-2004	61
F6102005	H-2005	61
F6102009	H-2006M	61
F6102025	H-2002.5	61
F6102301	K-2001	60
F6102303	K-2003	60
F6102304	K-2004	60
F6102305	K-2005	60
F6102306	K-2006	60
F6102309	K-2006M	60
F6102312	K-2002	60
F6102315	K-2002.5	60
F6102401	KF-2001	60
F6102402	KF-2002	60
F6102403	KF-2003	60
F6102404	KF-2004	60
F6102405	KF-2005	60
F6102406	KF-2006	60
F6102409	KF-2006M	60
F6102425	KF-2002.5	60
F6108010	KF-5001	61
F6108020	KF-5002	61
F6108025	KF-5002.5	61
F6108030	KF-5003	61
F6108040	KF-5004	61
F6110002	CM-825	72
F6110003	PH-814	74
F6110011	QA-825	70

Product Code	Product Name	Page
F6112100	DEAE3N-4T	70
F6112110	DEAE-2B	70
F6113000	SP-420N	72
F6113100	SP-FT 4A	72
F6113110	SP-2B	72
F6118250	SP-825	72
F6118255	DEAE-825	70
F6208390	AT-806MS	64
F6208600	UT-802.5	64
F6208610	UT-806M	64
F6208620	UT-807	64
F6208700	HT-803	64
F6208710	HT-804	64
F6208720	HT-805	64
F6208730	HT-806	64
F6208740	HT-806M	64
F6208770	HT-807	64
F6354211	P-421S	72
F6356240	WA-624	70
F6378010	KS-801	26
F6378020	KS-802	26
F6378025	KS-803	26
F6378030	KC-811	30
F6378033	KC-811 6E	30
F6378035	KS-804	26
F6378050	KS-805	26
F6378060	KS-806	26
F6378100	SH1011	26
F6378101	SH1821	26
F6378102	SC1011	26
F6378103	SC1821	26
F6378105	SP0810	26
F6379230	MN-431	27
F6379300	SC1011-7F	27
F6429100	SB-802 HQ	42
F6429101	SB-802.5 HQ	42
F6429102	SB-803 HQ	42
F6429103	SB-804 HQ	42
F6429104	SB-805 HQ	42
F6429105	SB-806 HQ	42
F6429106	SB-806M HQ	42
F6429108	SB-807 HQ	42
F6429201	LB-803	42
F6429202	LB-806M	42
F6429203	LB-805	42
F6502007	KS-2001	27
F6502008	KS-2002	27
F6502009	KS-2003	27
F6502010	KS-2004	27
F6502011	KS-2005	27
F6502012	KS-2006	27
F6505012	KC-2011	30
F6505020	KW-2002.5	39
F6505021	KW-2003	39
F6505022	KW-2004	39

Product Code	Product Name	Page
F6513013	DE-2013	13
F6514013	DC-2013	27
F6514014	DM-2014	13
F6516011	SB-2002	43
F6516012	SB-2002.5	43
F6516013	SB-2003	43
F6516014	SB-2004	43
F6516015	SB-2005	43
F6516016	SB-2006	43
F6516017	SB-2006M	43
F6548000	QA-2025	70
F6548001	DEAE-2025	70
F6548002	SP-2025	72
F6548003	CM-2025	72
F6650040	C18M 4D	22
F6650041	C18M 4E	22
F6650042	C18M 2D	22
F6650045	C18P 4D	22
F6650046	C18P 4E	22
F6650047	C18P 2D	22
F6650050	5SIL 4D	23
F6650051	5SIL 4E	23
F6650052	5C8 4D	22
F6650053	5C8 4E	22
F6650058	5CN 4D	22
F6650059	5CN 4E	22
F6650060	5NH 4D	23
F6650061	5NH 4E	23
F6650062	5NPE 4D	22
F6650063	5PYE 4D	22
F6651010	C18-4D	22
F6651011	C18-4E	22
F6700002	KS-G 8B (KS-LG)	27
F6700010	KC-G 8B (KC-LG)	30
F6700020	KS-G 6B (KS-G)	26
F6700030	KC-G 6B (KC-G)	30
F6700080	SH-G	30
F6700081	SP-G 6B (SP-G)	26
F6700090	SC-G 6B (SC-LG)	26,27
F6700100	HK-G filter	58
F6700110	SZ-G	26
F6700120	SC1211G 4A (SC-G)	26
F6700131	KW-G 6B (KW-G)	38
F6700132	KW400G-4A	39
F6700133	LW-G 6B	38

Product Code	Product Name	Page
F6700140	DS-G	12
F6700150	DE-G 4A (DE-G)	12
F6700151	DE-G 2A (DE-SG)	12
F6700160	DM-G 4A (DM-G)	12
F6700170	DC-G 4A (DC-G)	24
F6700190	DE-G 8B (DE-LG)	13
F6700200	HK-G	58
F6700210	P-G	72
F6700230	Y-G	34
F6700245	WA-G	70
F6700280	AT-G	64
F6700300	KF-G 4A (KF-G)	50,56
F6700310	H-G 8B (H-G)	61
F6700400	IA-G	32
F6700401	K-G 4A (K-G)	52
F6700402	DC-G 8B (DC-LG)	27
F6700404	DM-G 8B (DM-LG)	13
F6700406	KF-G 8B (KF-LG)	60
F6700407	K-G 8B (K-LG)	60
F6700408	KF-G 20C (KF-LLG)	61
F6700409	K-G 20C (K-LLG)	61
F6700411	KD-G 4A (KD-G)	54
F6700412	T-G	34
F6700500	HFIP-G 8B (HFIP-LG)	66
F6700510	NN-G	12
F6700511	HFIP-G 4A (HFIP-G)	66
F6700530	YS-G	34
F6709300	CRX-G	74
F6709350	KF-800D	50,54
F6709400	UT-G	64
F6709410	HT-G	64
F6709430	SB-G 6B (SB-G)	42
F6709431	SB-807G	42
F6709434	LB-G 6B	42
F6709450	K-800D	52,54
F6709555	SB-G 8B (SB-LG)	43
F6709556	KW-G 8B (KW-LG)	39

Product Code	Product Name	Page
F6709558	RP18-G	12
F6709602	QA-G 8B (QA-LG)	70
F6709603	DEAE-G 8B (DEAE-LG)	70
F6709604	SP-G 8B (SP-LG)	72
F6709605	CM-G 8B (CM-LG)	72
F6709608	YK-G	34
F6709616	NI-G	32
F6709620	SI-90G	32
F6709621	LF-G	62
F6709625	SI-50G	32
F6709626	SI-92G	32
F6709627	SI-95G	32
F6709720	SI-2GF	32
F6709730	SI-2GF filter	32
F6710001	ODP-50G 6A	10
F6710002	C8P-50G 4A	10
F6710003	C4P-50G 4A	10
F6710004	ODP-130G 7B	10
F6710016	NH2P-50G 4A	20
F6710017	NH2P-130G 7B	20
F6710018	GF-1G 7B	48
F6710019	GS-2G 7B	46
F6710020	GS-10G 7B	48
F6710021	GS-20G 7B	46,70,72
F6710022	ODP-50G 4A	10
F6710023	ODP-50 4B	10
F6710030	NH2P-50G 3A	20
F6710100	NH2P-LF	20
F6711100	VG-50G 4A	16
F6711200	VG-50G 2A	16
F6711300	VT-50G 2A	16
F6711400	VN-50G 4A	16
F6711500	VN-50G 2A	16
F6711600	VC-50G 2A	16
F6713000	NH2P-50G 2A	20
F6713001	ODP-50G 2A	10
F6714004	C8P-50G 7B	10
F6714005	C4P-50G 7B	10
F6714007	PAE-G	70
F6714008	PAE-G AC	70
F6714010	ODP2 HPG-4A	8
F6714011	ODP2 HPG-2A	8
F6714013	ODP-40G 3A	10
F6714014	ODP2 HPG-3A	8
F6714015	ODP2 HPG-7B	8
F6810017	GS-220 20F	42
F6810018	GS-320 20F	42
F6810019	GS-520 20F	42
F6810020	GS-620 20F	42
F6810022	PAE-2000	76

Product Code	Product Name	Page
F6810023	PAE-2000 AC	76
F6810030	GS-310 20F	48
F6810031	GS-510 20F	48
F6810032	GS-710 20F	48
F6810033	GSM-700 20F	48
F6810034	GS-220 20G	46
F6810035	GS-320 20G	46
F6810036	GS-520 20G	46
F6810037	GS-620 20G	46
F6810038	GS-310 20G	48
F6810039	GS-510 20G	48
F6810040	GS-710 20G	48
F6810041	GSM-700 20G	48
F6820001	ODP-50 10E	10
F6820003	C8P-50 10E	10
F6820005	C4P-50 10E	10
F6820035	ODP-90 20F	10
F6822001	ODP2 HP-10E	8
F6830001	NH2P-50 10E	20
F6830031	NH2P-90 20F	20
F6840003	ES-502C 20C	72
F6840004	ES-502N 20C	70
F6989000	KW-802.5	38
F6989103	KW-803	38
F6989104	KW-804	38
F6989201	KW402.5-4F	38
F6989202	KW403-4F	38
F6989203	KW404-4F	38
F6989204	KW405-4F	38
F6989303	LW-803	38
F6995210	Y-521	34
F6995240	I-524A	32
F6995243	NI-424	32
F6995244	SI-90 4E	32
F6995245	SI-50 4E	32
F6995250	T-521	34
F6995260	SI-52 4E	32
F6995290	SI-35 4D	32
F6995291	SI-35 2B	32
F7001001	DS-613	12
F7001002	DM-614	12
F7001003	DC-613	36
F7001004	DE-613	12
F7001005	DE-413	12
F7001007	DE-213	12
F7001012	DS-413	12
F7001300	SZ5532	26
F7001400	SC1211	26
F7008140	NN-814	12
F7008150	NN-614	12
F7008160	NN-414	12
F7008220	JJ-50 2D	12
F7008240	JJ-50 4D	12
F7009000	RP18-415	12
F7009030	DE-413L	12

Product Code	Product Name	Page
F7118946	APA-894	74
F7118964	ACH-494	74
F7120012	YK-421	34
F7122000	YS-50	34
F7140040	CRX-853	74
F7146003	CDBS-453	74
F7560040	C18M 10E	22
F7560041	C18M 20E	22
F7560050	5SIL 10E	23
F7560051	5SIL 20E	23
F7560060	5NH 10E	23
F7560061	5NH 20E	23
F7560062	5C8 10E	22
F7560063	5C8 20E	22
F7600000	GF-210 HQ	48
F7600001	GF-310 HQ	48
F7600002	GF-510 HQ	48
F7600003	GF-710 HQ	48
F7600004	GF-7M HQ	48
F7600005	GS-220 HQ	46
F7600006	GS-320 HQ	46
F7600007	GS-520 HQ	46
F7600008	GS-620 HQ	46
F7600024	GF-310 4E	48
F7600025	PAE-800	76
F7600026	PAE-800 AC	76
F7600100	GF-310 4B	48
F7600110	GF-310 4D	48
F7600120	GF-310 2D	48
F7600200	GF-210 4D	48
F7600201	GF-210 4E	48
F7620001	ODP-50 6E	10
F7620002	ODP-50 6D	10
F7620003	ODP-50 4E	10
F7620004	ODP-50 4D	10
F7620005	C8P-50 4E	10
F7620006	C8P-50 4D	10
F7620007	C4P-50 4E	10
F7620008	C4P-50 4D	10
F7620009	ODP-50 2D	10
F7621001	ODP-40 4D	10
F7621002	ODP-40 4E	10
F7621101	ODP-40 3B	10
F7621102	ODP-40 3D	10
F7622001	ODP2 HP-4B	8
F7622002	ODP2 HP-4D	8
F7622003	ODP2 HP-4E	8
F7622004	ODP2 HP-2B	8
F7622005	ODP2 HP-2D	8
F7622006	ODP2 HP-3B	8
F7622007	ODP2 HP-3D	8
F7623001	ET-RP1 4D	74
F7630001	NH2P-50 4E	20
F7630002	NH2P-50 4D	20
F7630005	NH2P-50 4B	20

Product Code	Product Name	Page
F7630006	NH2P-50 2D	20
F7630007	NH2P-40 3E	20
F7630008	NH2P-40 2B	20
F7630009	NH2P-40 2D	20
F7630010	NH2P-40 2E	20
F7630011	NH2P-40 3B	20
F7630012	NH2P-40 3D	20
F7630100	VG-50 4E	16
F7630200	VG-50 4D	16
F7630300	VG-50 2D	16
F7630400	VT-50 2D	16
F7630500	VN-50 4D	16
F7630600	VN-50 2D	16
F7630700	VC-50 2D	16
F7640001	ES-502C 7C	72
F7640002	ES-502N 7C	70
F7750311	GS320A-4E	46
F7750312	GS320A-4D	46
F7760511	GF510A-4E	48
F7760512	GF510A-4D	48
F7838022	ODP40-2D	8
F7838023	ODP40-2B	8
F7840121	DE413-2E	13
F7840123	DE413-2B	13
F7860122	NN414-2D	13
F8400000	P-82	69
F8400005	P-5	69
F8400010	P-10	69
F8400020	P-20	69
F8400050	P-50	69
F8400100	P-100	69
F8400200	P-200	69
F8400400	P-400	69
F8400800	P-800	69
F8500630	FL-1	32,34
F8500640	FL-1 filter	32,34
F8601105	SL-105	69
F8602105	SM-105	69
F8603075	SH-75	69
F8604075	M-75	69
F8700015	GF-4A	74



We provide a wide range of products to meet your analytical needs, from pretreatment and separation columns to calibration standards for size exclusion chromatography.

Please visit the Shodex website to see detailed information about our products and their uses with abundant application data.

Shodex website

www.shodex.de



The following names are trademarks or registered trademarks of SHOWA DENKO K.K.

Shodex, AFpak, Asahipak, AXpak, CLNpak, CXpak, HILICpak, MSPak, ODP, OHpak, ORpak, RSpak, SUGAR, USPpak

[Caution]

1. Please read the operating manual packaged with the product carefully before the use.
2. For improvement purposes, some specifications are subject to change without notice.
3. Figures and descriptions in this catalogue are provided to help you select appropriate columns. However they do not guarantee nor warrant the suitability for your applications.
4. It is essential to take normal precautions when handling reagents and other chemical products even if the safety information is not included in the operating manual.
5. Products described in this brochure are not intended for medical use or medical applications including medical diagnosis.

**You can receive support by Shodex worldwide.
Languages other than English are available now.
Please contact Shodex website of your area.**

■ Showa Denko Europe GmbH

Service area : Europe Africa Middle East Russia

Correspondence language : German English Spanish

URL www.shodex.de

■ Showa Denko K.K.

Service area : Taiwan

Correspondence language : Japanese English

URL www.shodex.com



■ Shoko Co., Ltd.

Service area : Japan

Correspondence language : Japanese

URL www.shodex.com/ja

■ Shoko Korea Co., Ltd.

Service area : Korea

Correspondence language : Korean (Hangul alphabet)

URL www.shodex.com/kr

■ Showa Denko America, Inc.

Service area : North America Latin America

Correspondence language : English French Spanish Portuguese

URL www.shodexhplc.com

■ Showa Denko Singapore (Pte) Ltd.

Service area : Southeast Asia India Oceania

Correspondence language : English

URL www.sds.com.sg

■ Shodex China Co., Ltd.

Service area : China Hong Kong Macau

Correspondence language : Chinese (Simplified Chinese character)

URL www.shodex.com/cn

Please contact a Shodex support office near you

Support office

Europe**Africa****Middle East****Russia****Showa Denko Europe GmbH**

Konrad-Zuse-Platz 3 D-81829 Munich, Germany

Tel: +49 (0)89 93 99 62-37 Fax: +49 (0)89 93 99 62-7734

E-mail: order@shodex.deURL: <http://www.shodex.de/>**Southeast Asia****India****Oceania****Showa Denko Singapore (Pte) Ltd.**

2 Shenton Way #15-03/04, SGX Centre 1, Singapore 068804

Tel: +65-6223-1889

E-mail: sds-admi@sds.com.sgURL: <http://www.sds.com.sg/>**Taiwan****Showa Denko K.K.**

13-9 Shiba Daimon 1-chome, Minato-ku, Tokyo 105-8518, Japan

Tel: +81 (0)3 6402 5140 Fax: +81 (0)3 5403 5730

E-mail: Sdk_shodex@showadenko.comURL: <http://www.shodex.com/en/>**China****Hong Kong****Macau****Shodex China Co., Ltd.**

18F, No.211 Shi Men Yi Road, Jing An, Shanghai, 200041, China

Tel: +86 (0)21 6217-6111 Fax: +86 (0)21 6217-9879

E-mail: sales@shodexchina.comURL: <http://www.shodex.com/cn/>**Korea****Shoko Korea Co., Ltd.**

#322, Chungjeong Rizion, 27, Seosomun-ro, Seodaemun-gu, Seoul 03741, Korea

Tel: +82 (0)2 784 5111 Fax: +82 (0)2 784 5125

E-mail: shoko.korea@shokokorea.comURL: <http://www.shodex.com/kr/>**Japan****SHOKO SCIENCE Co., Ltd.**

4-1, Shibakoen 2-chome, Minato-ku, Tokyo, 105-8432, Japan

Tel: +81 3 3459 5104 Fax: +81 3 3459 5081

E-mail: shodex.tokyo@shoko.co.jpURL: <http://www.shodex.com/ja/>**North America****Latin America****Showa Denko America, Inc.**

420 Lexington Avenue Suite 2335A, New York, NY 10170 USA

Tel: +1 212 370 0033 Fax: +1 212 370 4566

E-mail: sales@shodexhplc.comURL: <http://www.shodexhplc.com/>**www.shodex.de**

Manufactured by

**SHOWA DENKO K.K.****Shodex (Separation & HPLC) Group**

13-9 Shiba Daimon 1-chome, Minato-ku, Tokyo 105-8518, Japan

Tel: +81 (0)3 6402 5140 Fax: +81 (0)3 5403 5730



КОМПЛЕКСНОЕ ОСНАЩЕНИЕ
+7(916)414-93-61 www.sov-lab.ru
+7(495)045-58-29 sov_lab@mail.ru